

Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD062321\
 Data File : VD069546.D
 Acq On : 23 Jun 2021 15:45
 Operator : VA/SY
 Sample : M2773-02
 Misc : 5.13G/5.00ml/MSVOA_D/SOIL
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_D
 ClientSampleId :
 SB-2

Quant Time: Jun 24 06:09:27 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D062121S.M
 Quant Title : SW846 8260
 QLast Update : Tue Jun 22 04:33:24 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	7.979	168	445844	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	8.861	114	885220	50.00	ug/l	0.00
63) Chlorobenzene-d5	11.643	117	936499	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.567	152	425813	50.00	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.332	65	367396	66.11	ug/l	0.00
Spiked Amount	50.000	Range	50 - 163	Recovery	=	132.22%
35) Dibromofluoromethane	7.914	113	319779	53.44	ug/l	0.00
Spiked Amount	50.000	Range	54 - 147	Recovery	=	106.88%
50) Toluene-d8	10.337	98	1169402	52.10	ug/l	0.00
Spiked Amount	50.000	Range	49 - 140	Recovery	=	104.20%
62) 4-Bromofluorobenzene	12.625	95	428278	58.04	ug/l	0.00
Spiked Amount	50.000	Range	25 - 144	Recovery	=	116.08%


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD062321\
Data File : VD069546.D
Acq On : 23 Jun 2021 15:45
Operator : VA/SY
Sample : M2773-02
Misc : 5.13G/5.00ml/MSVOA_D/SOIL
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
SB-2

Quant Time: Jun 24 06:09:27 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D062121S.M
Quant Title : SW846 8260
QLast Update : Tue Jun 22 04:33:24 2021
Response via : Initial Calibration



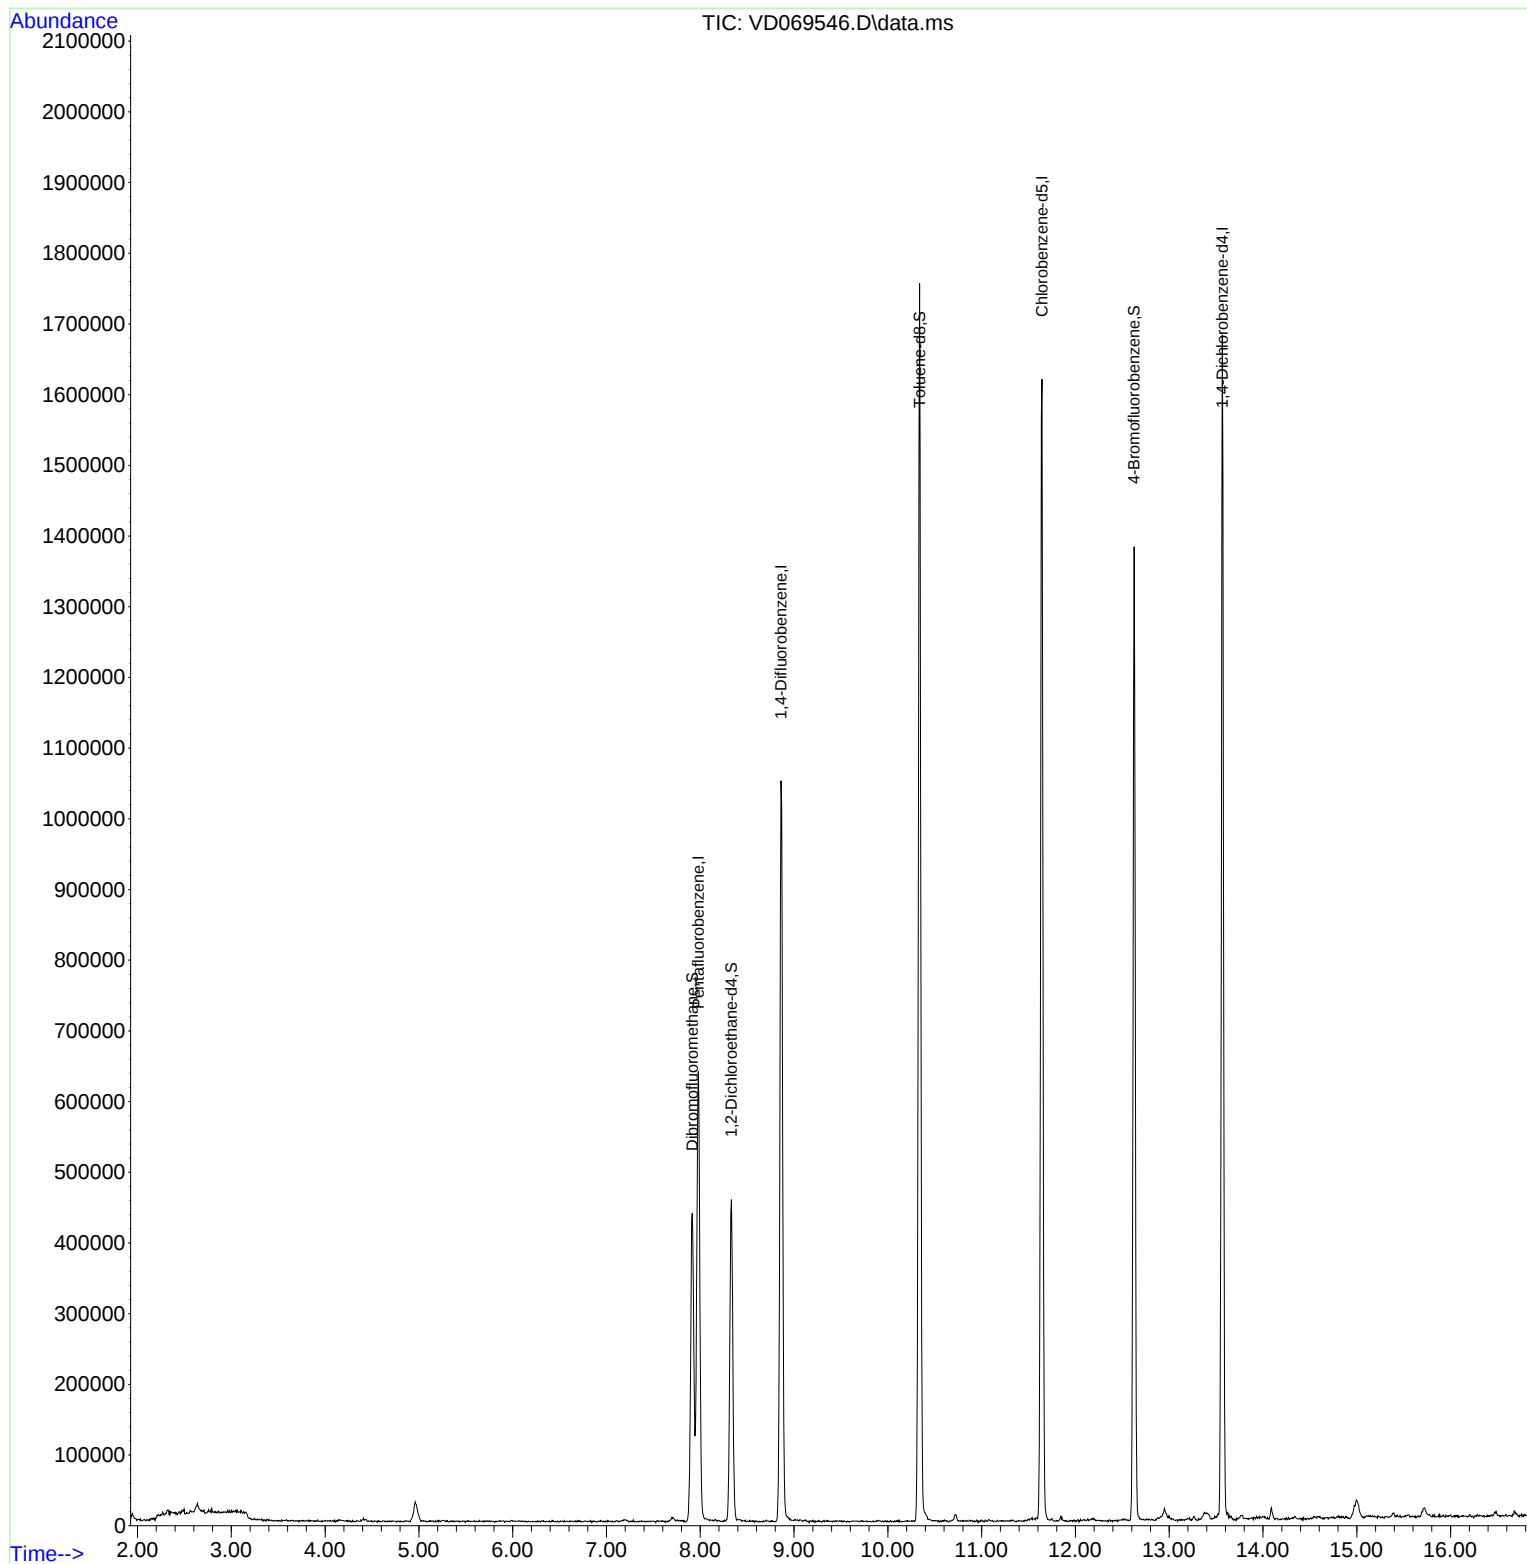


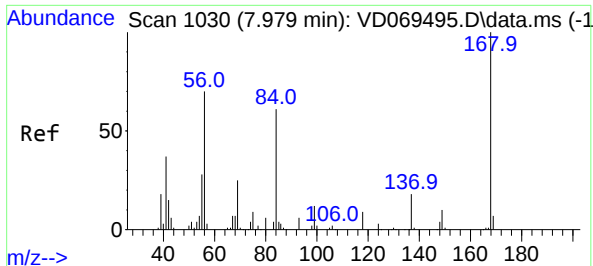

#1
Pentafluorobenzene
Concen: 50.00 ug/l
RT: 7.979 min Scan# 1030
Delta R.T. -0.000 min
Lab File: VD069546.D
Acq: 23 Jun 2021 15:45




Instrument :
MSVOA_D
ClientSampleId :
SB-2


Tgt Ion:168 Resp: 445844
Ion Ratio Lower Upper
168 100
99 58.5 49.3 73.9

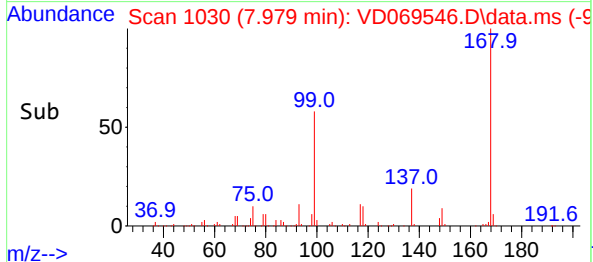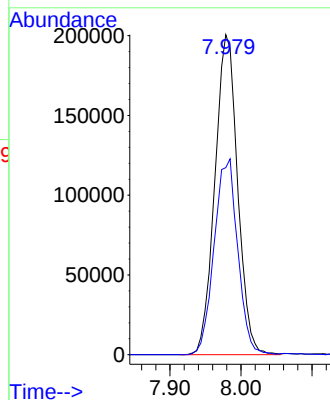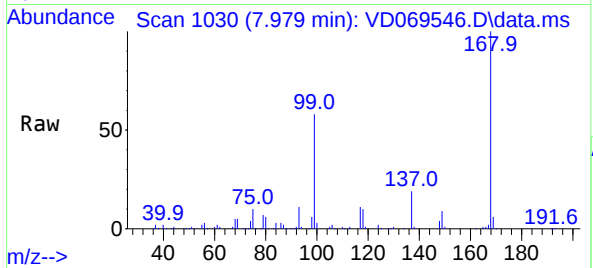

#33
1,2-Dichloroethane-d4
Concen: 66.11 ug/l
RT: 8.332 min Scan# 1090
Delta R.T. -0.000 min
Lab File: VD069546.D
Acq: 23 Jun 2021 15:45

Tgt Ion: 65 Resp: 367396
Ion Ratio Lower Upper
65 100
67 52.8 0.0 105.6

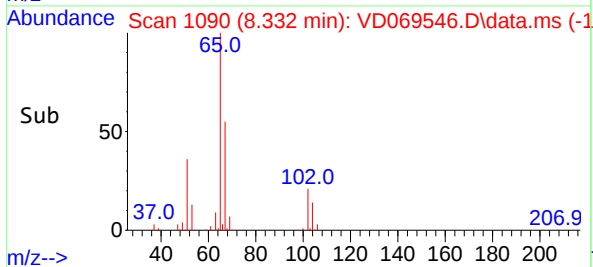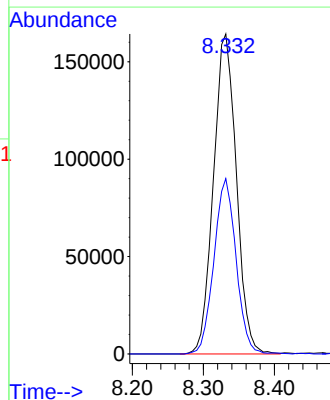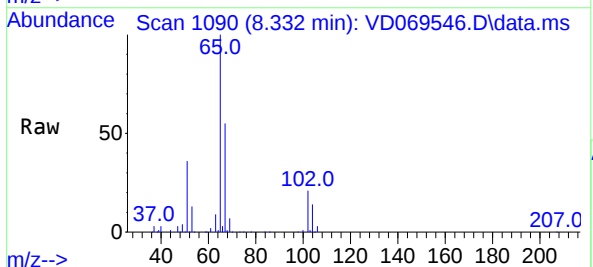

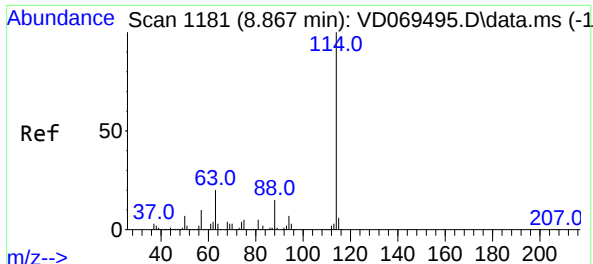





#34

1,4-Difluorobenzene
Concen: 50.00 ug/l
RT: 8.861 min Scan# 1180
Delta R.T. -0.006 min
Lab File: VD069546.D
Acq: 23 Jun 2021 15:45

Instrument :
MSVOA_D
ClientSampleId :
SB-2

Tgt Ion:114 Resp: 885220

Ion	Ratio	Lower	Upper
114	100		
63	21.6	0.0	39.6
88	15.8	0.0	29.8

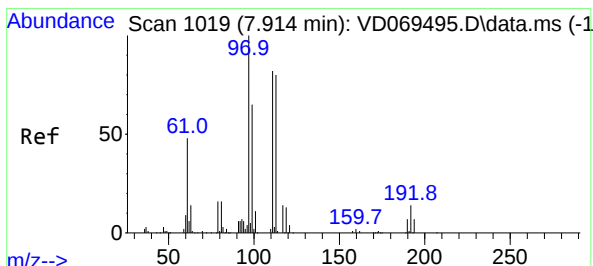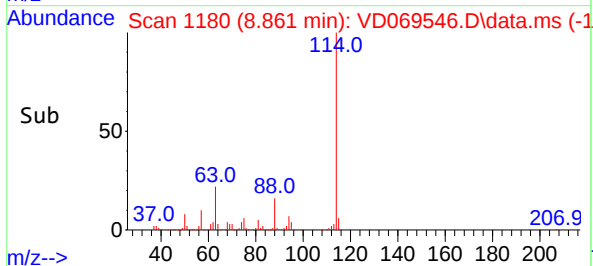
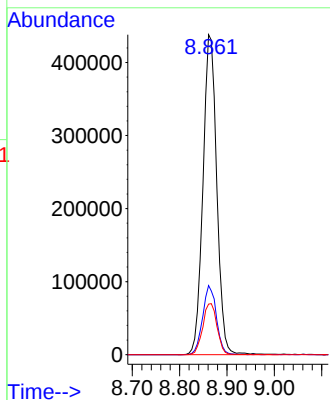
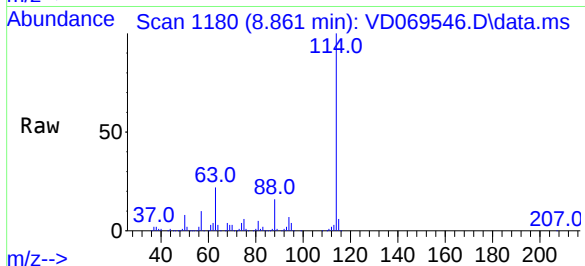



#35

Dibromofluoromethane
Concen: 53.44 ug/l
RT: 7.914 min Scan# 1019
Delta R.T. -0.000 min
Lab File: VD069546.D
Acq: 23 Jun 2021 15:45

Tgt Ion:113 Resp: 319779

Ion	Ratio	Lower	Upper
113	100		
111	102.3	81.8	122.8
192	16.5	13.8	20.6


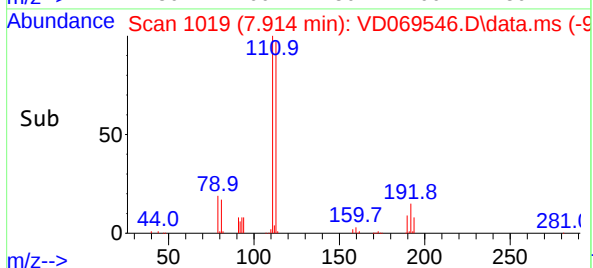
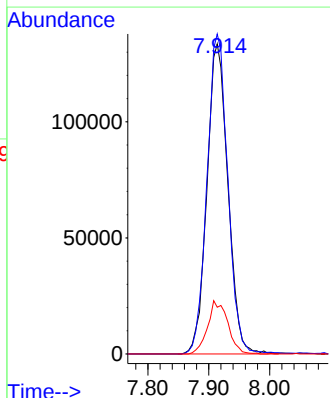
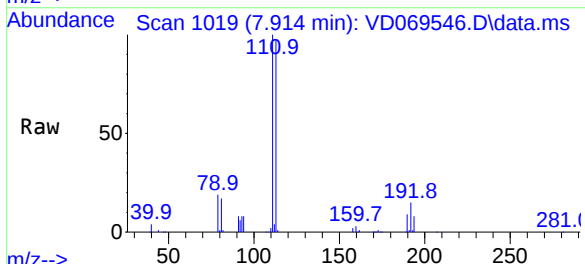


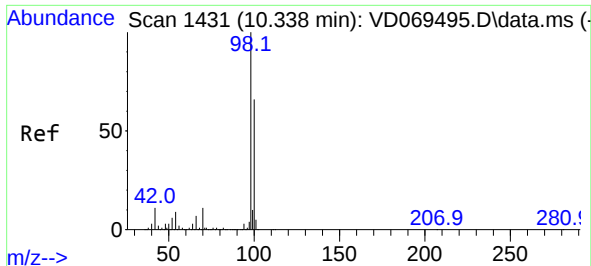

#50
Toluene-d8
Concen: 52.10 ug/l
RT: 10.337 min Scan# 1431
Delta R.T. -0.000 min
Lab File: VD069546.D
Acq: 23 Jun 2021 15:45




Instrument :
MSVOA_D
ClientSampleId :
SB-2


Tgt Ion: 98 Resp: 1169402
Ion Ratio Lower Upper
98 100
100 63.6 52.3 78.5

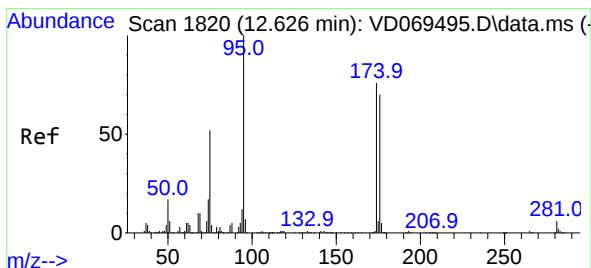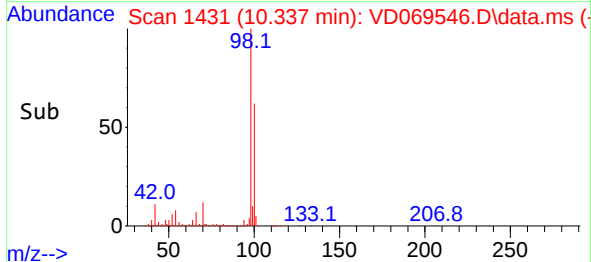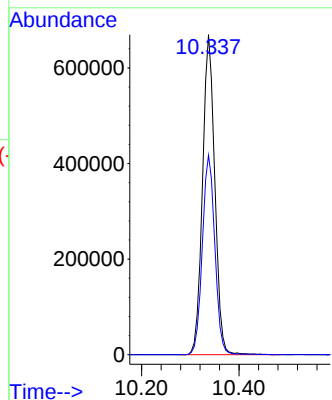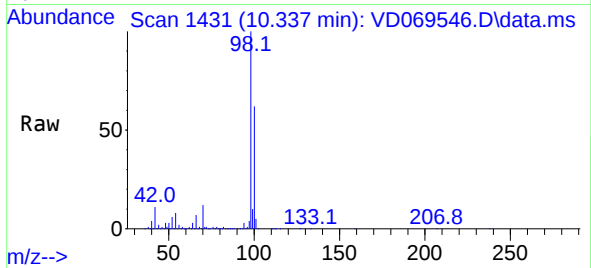

#62
4-Bromofluorobenzene
Concen: 58.04 ug/l
RT: 12.625 min Scan# 1820
Delta R.T. -0.000 min
Lab File: VD069546.D
Acq: 23 Jun 2021 15:45

Tgt Ion: 95 Resp: 428278
Ion Ratio Lower Upper
95 100
174 72.5 0.0 148.0
176 69.9 0.0 139.8


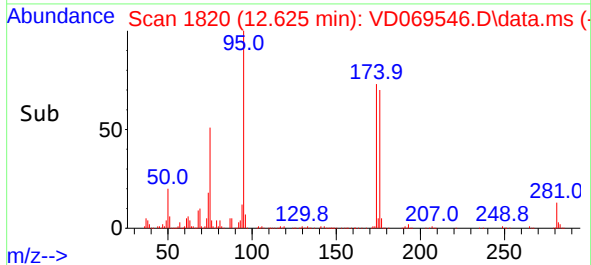
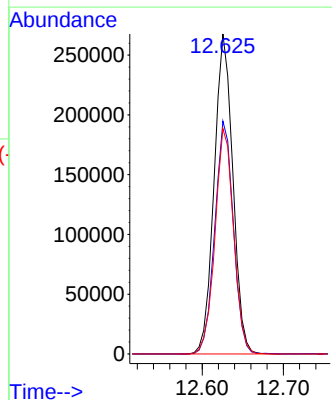
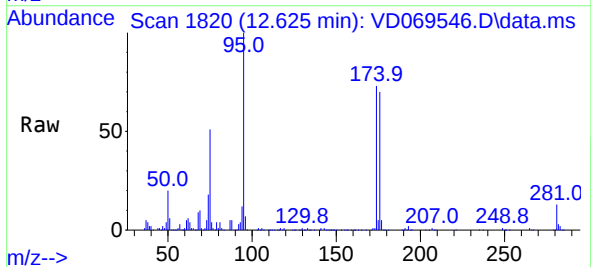


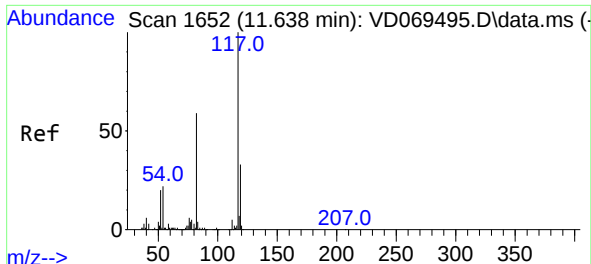

#63
Chlorobenzene-d5
Concen: 50.00 ug/l
RT: 11.643 min Scan# 1653
Delta R.T. 0.005 min
Lab File: VD069546.D
Acq: 23 Jun 2021 15:45

Instrument :
MSVOA_D
ClientSampled :
SB-2

Tgt Ion:117 Resp: 936499
Ion Ratio Lower Upper
117 100
82 56.3 46.8 70.2
119 32.2 26.2 39.2

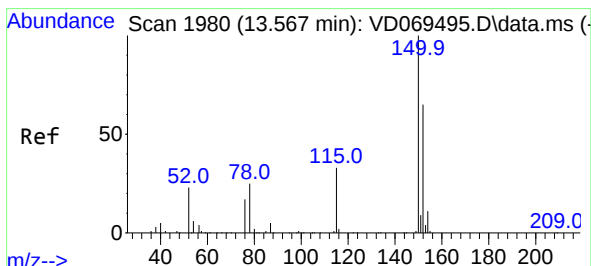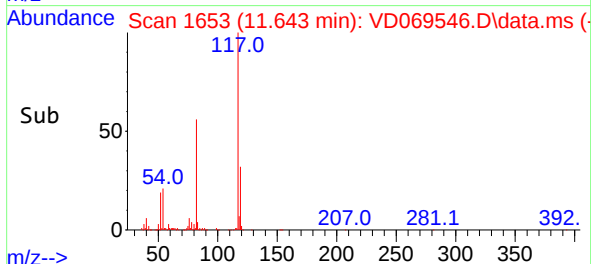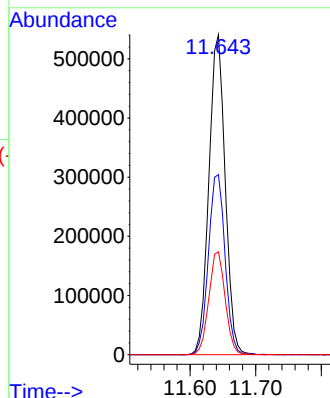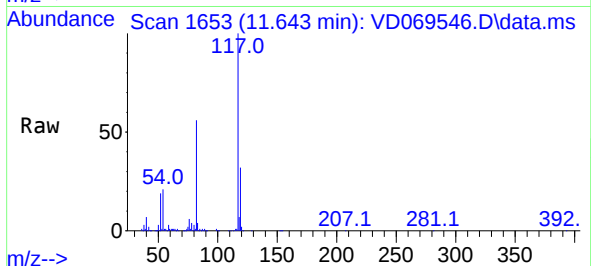

#72
1,4-Dichlorobenzene-d4
Concen: 50.00 ug/l
RT: 13.567 min Scan# 1980
Delta R.T. -0.000 min
Lab File: VD069546.D
Acq: 23 Jun 2021 15:45

Tgt Ion:152 Resp: 425813
Ion Ratio Lower Upper
152 100
115 63.3 31.7 95.1
150 158.1 0.0 350.8

