
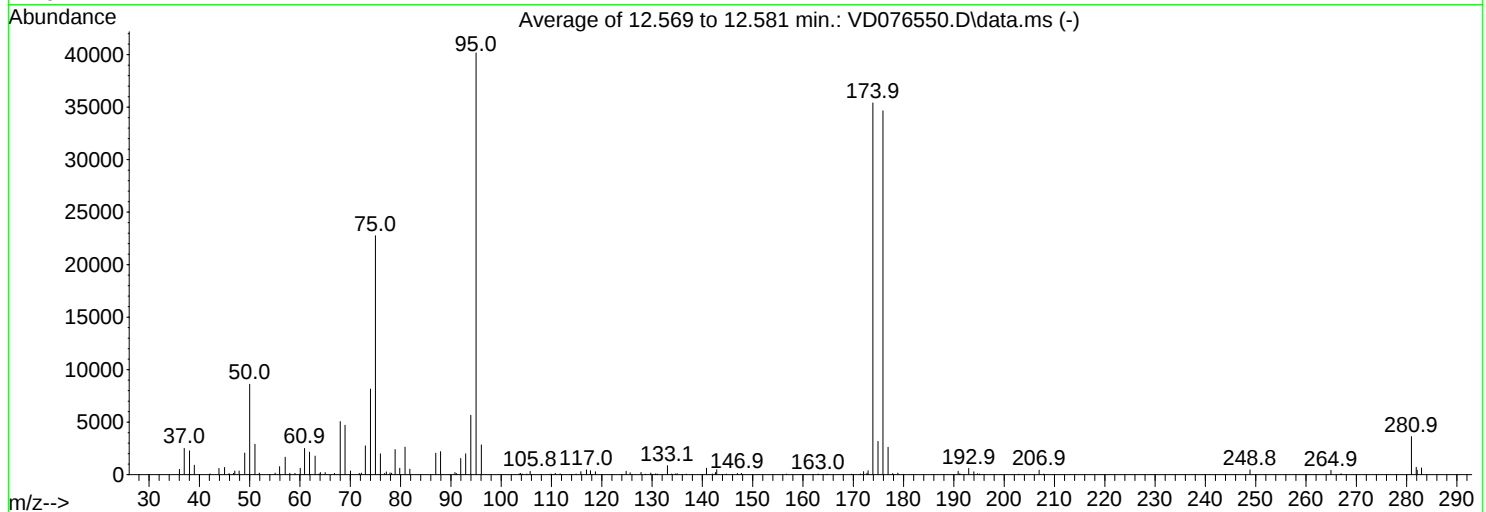


Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD062323\
Data File : VD076550.D
Acq On : 23 Jun 2023 10:33
Operator : KP/SY
Sample : BFB
Misc : 5.00G/5.0ml/MSVOA_D/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D061623S.M
Title : SW846 8260
Last Update : Mon Jun 19 04:51:45 2023

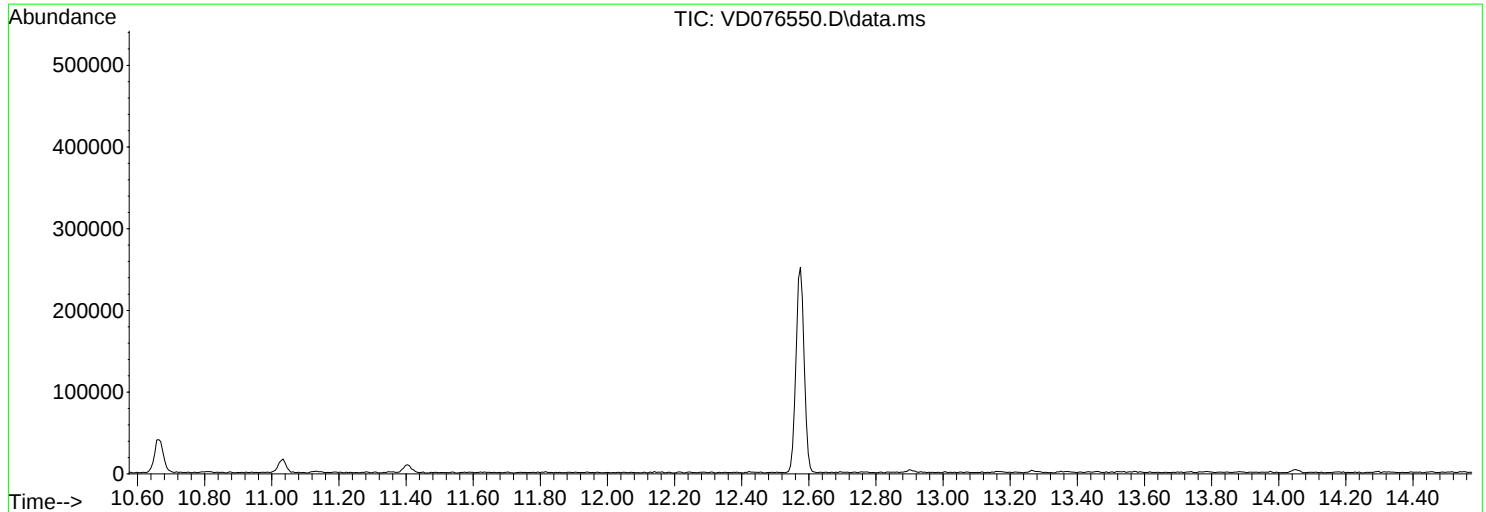

AutoFind: Scans 1867, 1868, 1869; Background Corrected with Scan 1859

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	21.4	8614	PASS
75	95	30	60	56.6	22749	PASS
95	95	100	100	100.0	40171	PASS
96	95	5	9	7.1	2841	PASS
173	174	0.00	2	1.1	382	PASS
174	95	50	100	88.1	35400	PASS
175	174	5	9	9.0	3173	PASS
176	174	95	101	97.9	34659	PASS
177	176	5	9	7.5	2609	PASS