
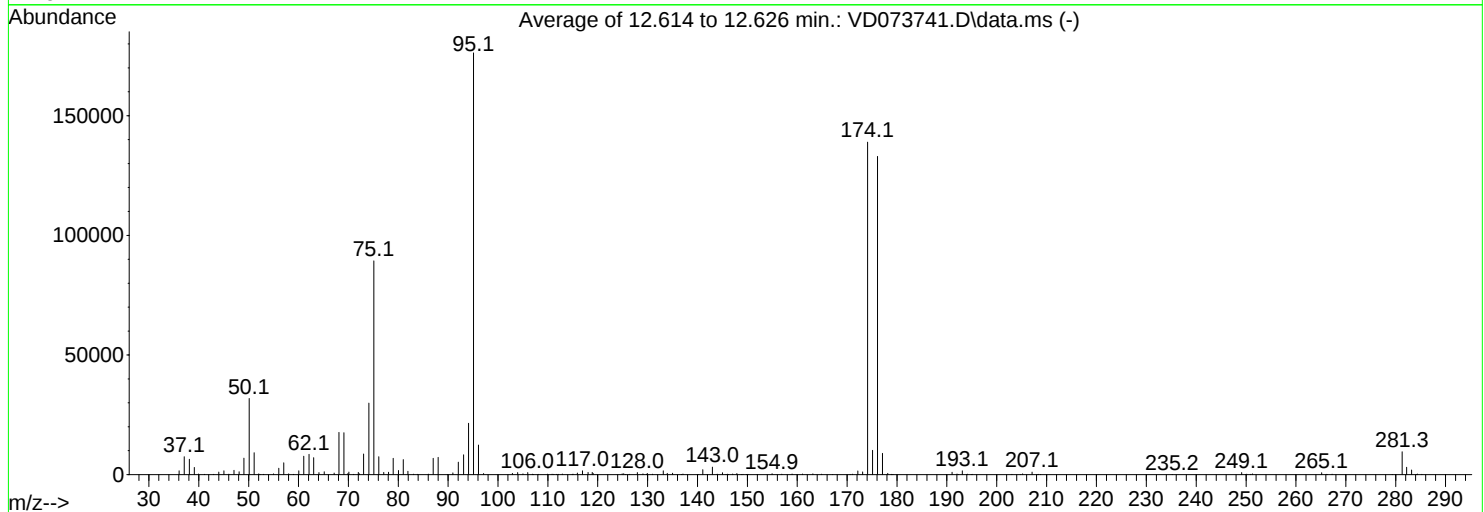


Data Path : Z:\voasrv\HPCHEM1\MSVOA\_D\Data\VD062822\  
Data File : VD073741.D  
Acq On : 28 Jun 2022 09:01  
Operator : VA/SY  
Sample : BFB  
Misc : 5.00G/5.00ml/MSVOA\_D/SOIL  
ALS Vial : 1 Sample Multiplier: 1

Instrument :  
MSVOA\_D  
ClientSampleId :  
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA\_D\Method\82D062722S.M  
Title : SW846 8260  
Last Update : Mon Jun 27 16:20:04 2022

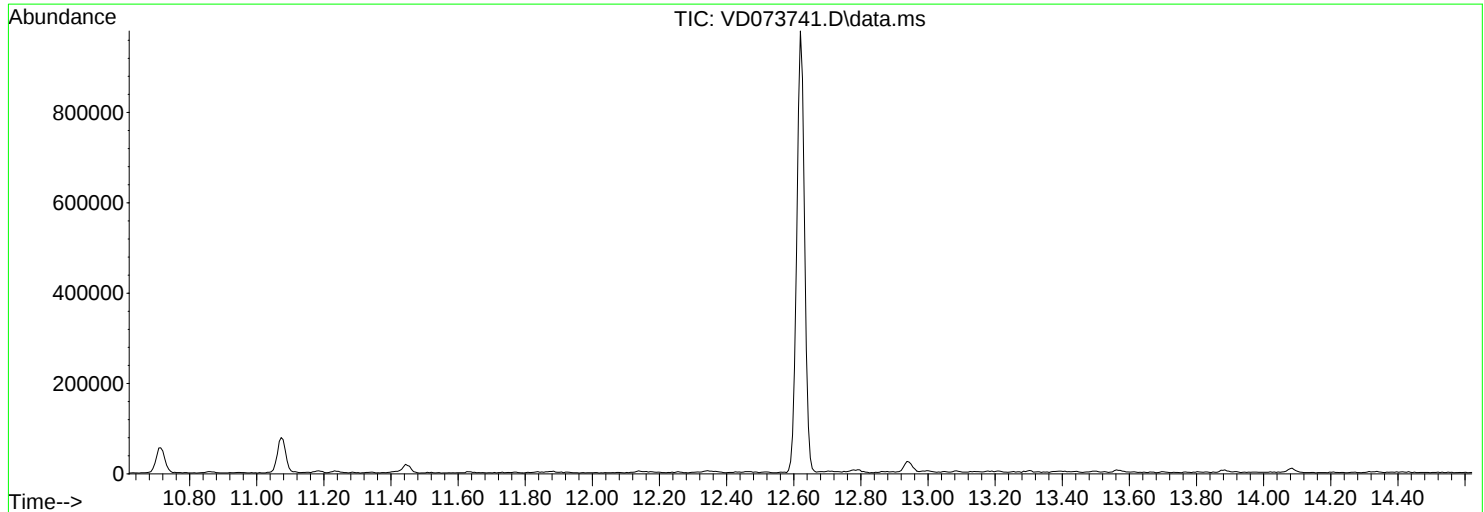

AutoFind: Scans 1818, 1819, 1820; Background Corrected with Scan 1806

| Target | Rel. to | Lower  | Upper  | Rel.  | Raw    | Result    |
|--------|---------|--------|--------|-------|--------|-----------|
| Mass   | Mass    | Limit% | Limit% | Abn%  | Abn    | Pass/Fail |
| 50     | 95      | 15     | 40     | 18.1  | 31824  | PASS      |
| 75     | 95      | 30     | 60     | 50.7  | 89307  | PASS      |
| 95     | 95      | 100    | 100    | 100.0 | 176277 | PASS      |
| 96     | 95      | 5      | 9      | 7.0   | 12361  | PASS      |
| 173    | 174     | 0.00   | 2      | 0.8   | 1123   | PASS      |
| 174    | 95      | 50     | 100    | 78.8  | 138963 | PASS      |
| 175    | 174     | 5      | 9      | 7.3   | 10190  | PASS      |
| 176    | 174     | 95     | 101    | 95.7  | 133035 | PASS      |
| 177    | 176     | 5      | 9      | 6.7   | 8918   | PASS      |