
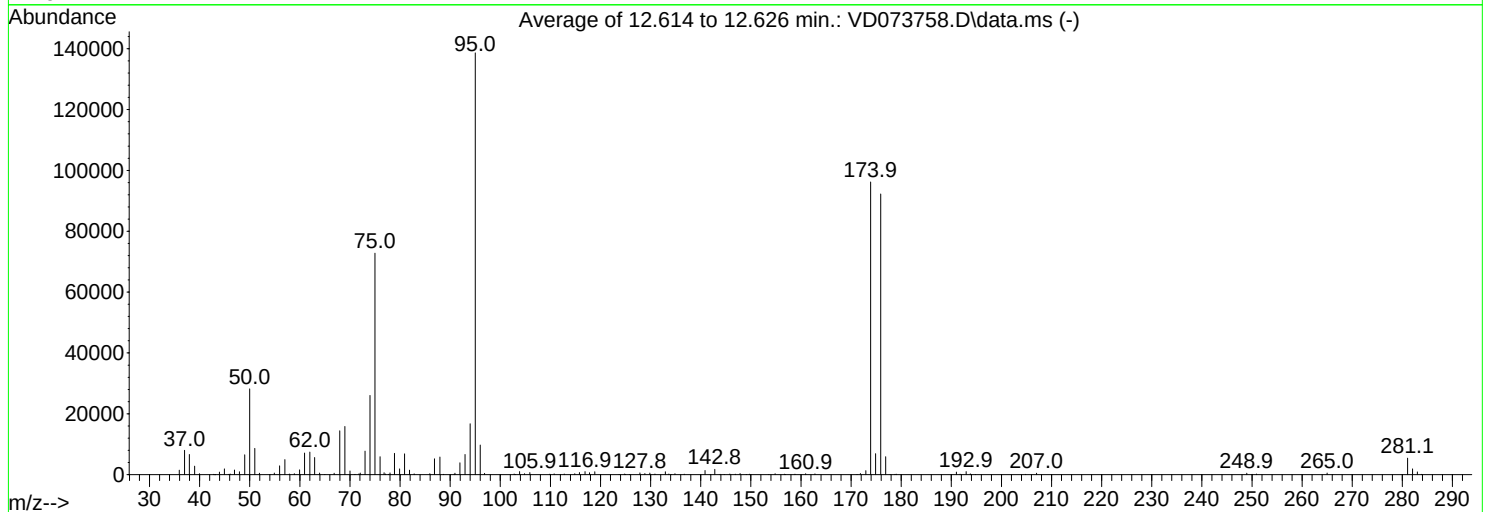


Data Path : Z:\voasrv\HPCHEM1\MSVOA\_D\Data\VD070122\  
Data File : VD073758.D  
Acq On : 01 Jul 2022 07:42  
Operator : VA/SY  
Sample : BFB  
Misc : 5.00G/5.00ml/MSVOA\_D/SOIL  
ALS Vial : 1 Sample Multiplier: 1

Instrument :  
MSVOA\_D  
ClientSampleId :  
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA\_D\Method\82D063022S.M  
Title : SW846 8260  
Last Update : Tue Jul 05 10:05:34 2022

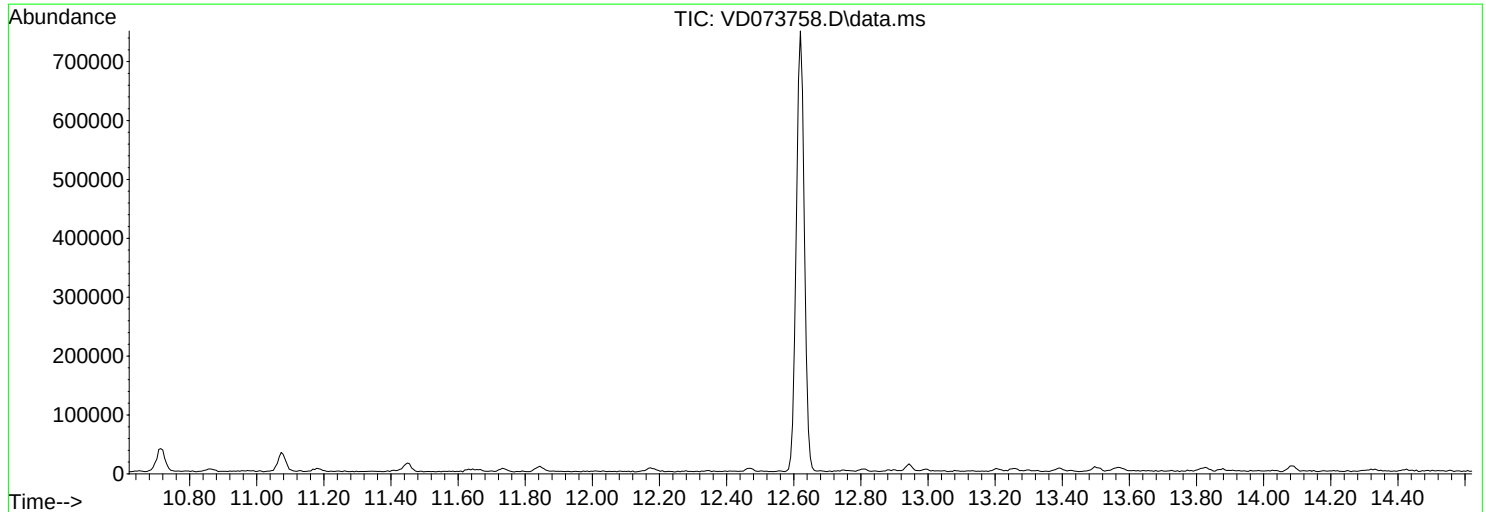

AutoFind: Scans 1818, 1819, 1820; Background Corrected with Scan 1809

| Target | Rel. to | Lower  | Upper  | Rel.  | Raw    | Result    |
|--------|---------|--------|--------|-------|--------|-----------|
| Mass   | Mass    | Limit% | Limit% | Abn%  | Abn    | Pass/Fail |
| 50     | 95      | 15     | 40     | 20.3  | 28213  | PASS      |
| 75     | 95      | 30     | 60     | 52.5  | 72787  | PASS      |
| 95     | 95      | 100    | 100    | 100.0 | 138645 | PASS      |
| 96     | 95      | 5      | 9      | 7.0   | 9747   | PASS      |
| 173    | 174     | 0.00   | 2      | 1.4   | 1330   | PASS      |
| 174    | 95      | 50     | 100    | 69.4  | 96184  | PASS      |
| 175    | 174     | 5      | 9      | 7.2   | 6889   | PASS      |
| 176    | 174     | 95     | 101    | 95.9  | 92256  | PASS      |
| 177    | 176     | 5      | 9      | 6.4   | 5918   | PASS      |