

Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD070522\
 Data File : VD073779.D
 Acq On : 05 Jul 2022 17:35
 Operator : VA/SY
 Sample : N3562-09RE
 Misc : 6.05G/5.00ml/MSVOA_D/SOIL
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_D
 ClientSampleId :
 SB-11ARE

Quant Time: Jul 06 02:51:41 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D063022S.M
 Quant Title : SW846 8260
 QLast Update : Tue Jul 05 10:05:34 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	7.967	168	106958	50.000	ug/l	# 0.00
34) 1,4-Difluorobenzene	8.855	114	217350	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.632	117	152265	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.561	152	36997	50.000	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.320	65	67647	64.833	ug/l	0.00
Spiked Amount	50.000	Range	50 - 163	Recovery	=	129.660%
35) Dibromofluoromethane	7.908	113	66018	55.913	ug/l	0.00
Spiked Amount	50.000	Range	54 - 147	Recovery	=	111.820%
50) Toluene-d8	10.332	98	165438	38.197	ug/l	0.00
Spiked Amount	50.000	Range	78 - 12	Recovery	=	76.400%#
62) 4-Bromofluorobenzene	12.620	95	51487	30.139	ug/l	0.00
Spiked Amount	50.000	Range	50 - 14	Recovery	=	60.280%#


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD070522\
Data File : VD073779.D
Acq On : 05 Jul 2022 17:35
Operator : VA/SY
Sample : N3562-09RE
Misc : 6.05G/5.00ml/MSVOA_D/SOIL
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
SB-11ARE

Quant Time: Jul 06 02:51:41 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D063022S.M
Quant Title : SW846 8260
QLast Update : Tue Jul 05 10:05:34 2022
Response via : Initial Calibration




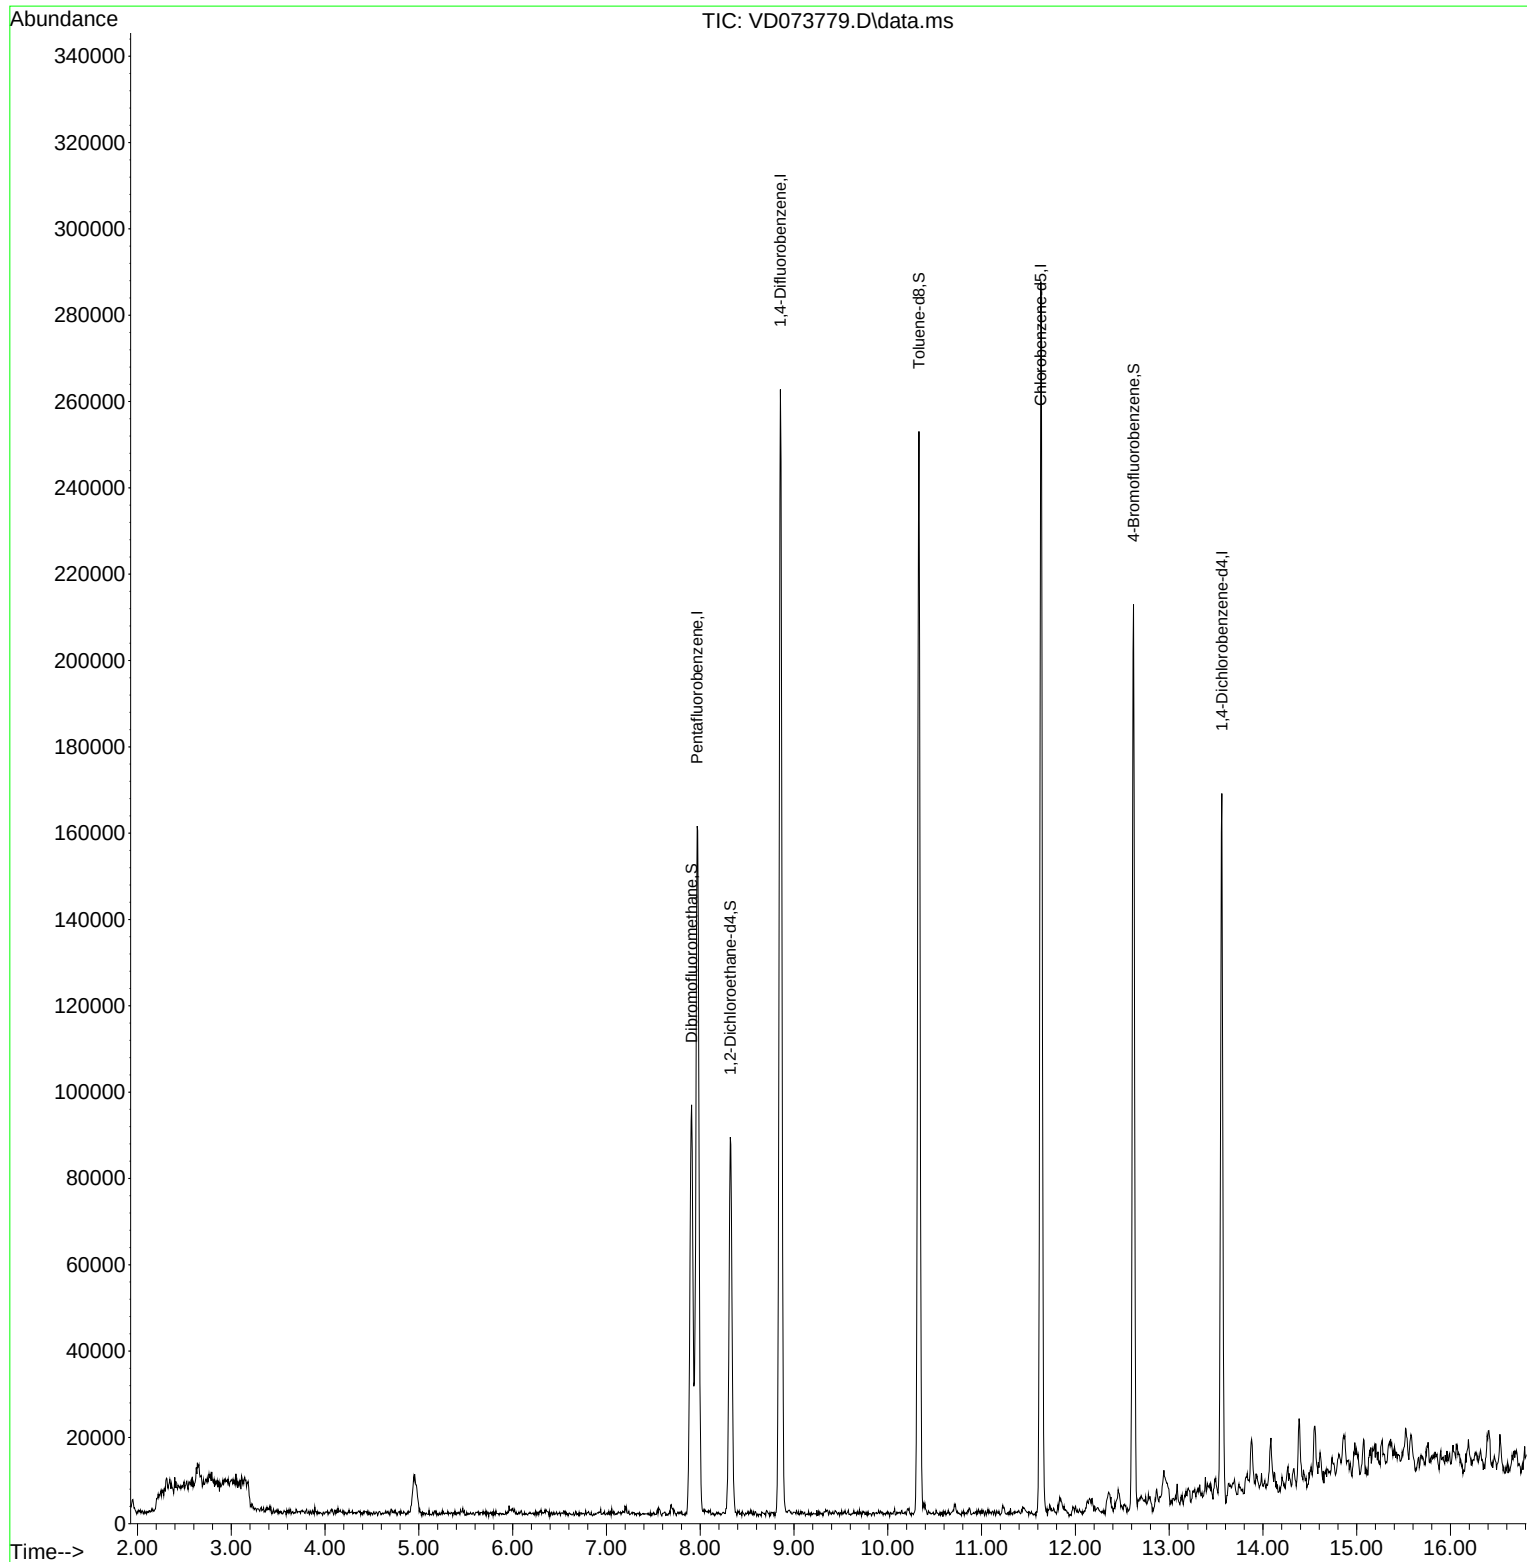


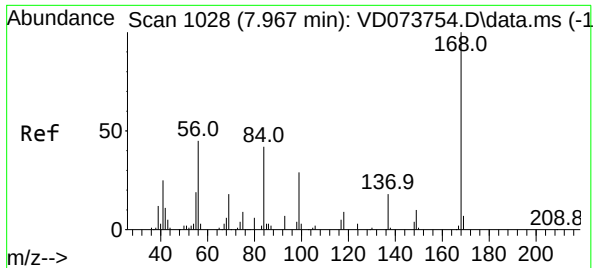

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 7.967 min Scan# 1028
Delta R.T. 0.000 min
Lab File: VD073779.D
Acq: 05 Jul 2022 17:35




Instrument :
MSVOA_D
ClientSampleId :
SB-11ARE


Tgt Ion:168 Resp: 106958
Ion Ratio Lower Upper
168 100
99 71.9 46.4 69.6#

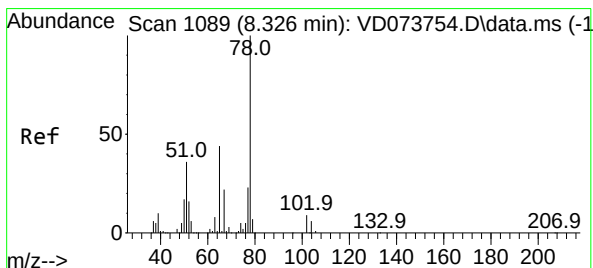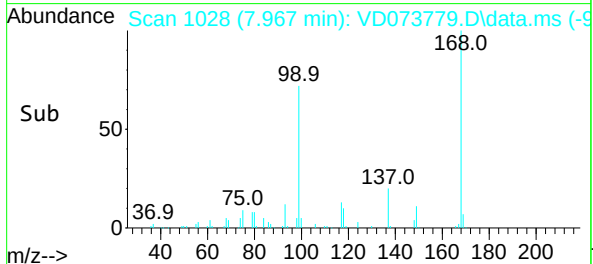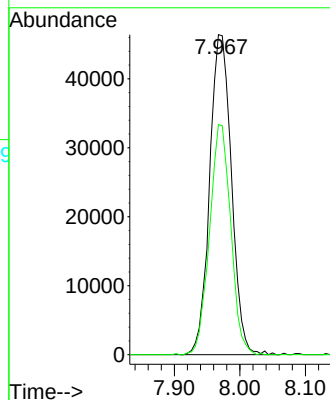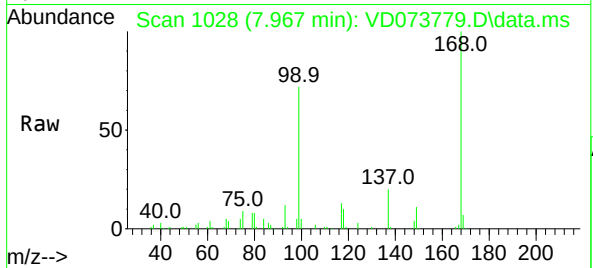

#33
1,2-Dichloroethane-d4
Concen: 64.833 ug/l
RT: 8.320 min Scan# 1088
Delta R.T. -0.006 min
Lab File: VD073779.D
Acq: 05 Jul 2022 17:35

Tgt Ion: 65 Resp: 67647
Ion Ratio Lower Upper
65 100
67 52.2 0.0 107.2

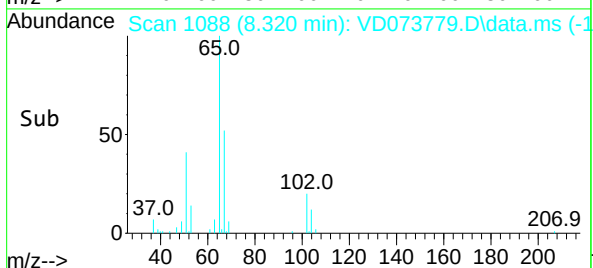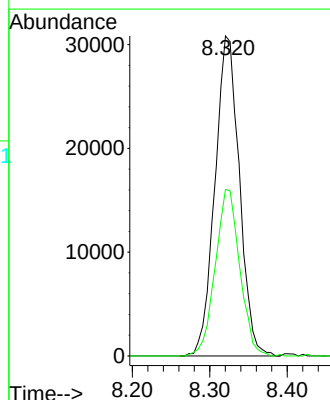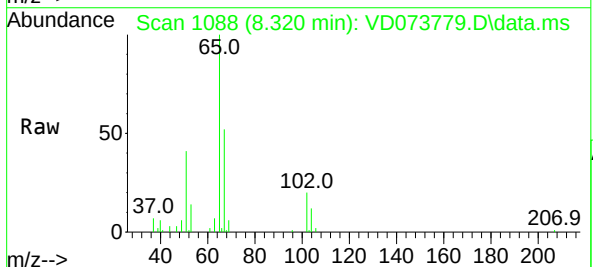

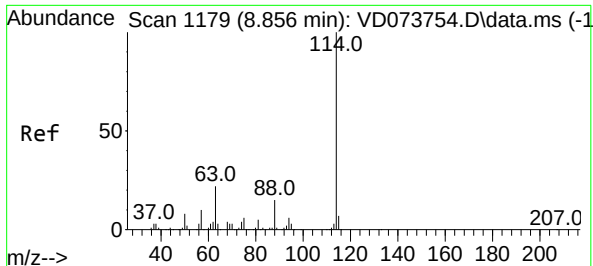

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 8.855 min Scan# 1179

Delta R.T. -0.000 min

Lab File: VD073779.D

Acq: 05 Jul 2022 17:35

Instrument :

MSVOA_D

ClientSampleId :

SB-11ARE





Tgt Ion:114 Resp: 217350

Ion Ratio Lower Upper

114 100

63 20.9 0.0 39.2

88 16.3 0.0 29.4

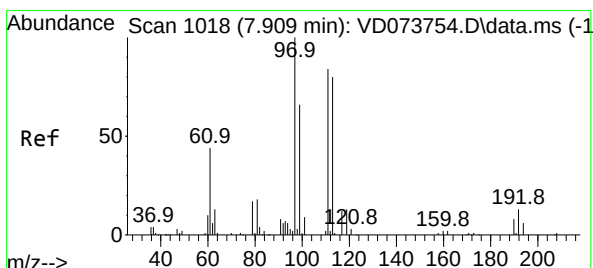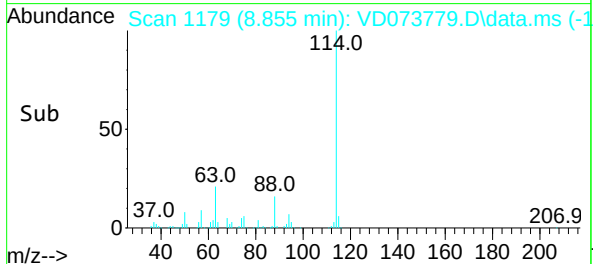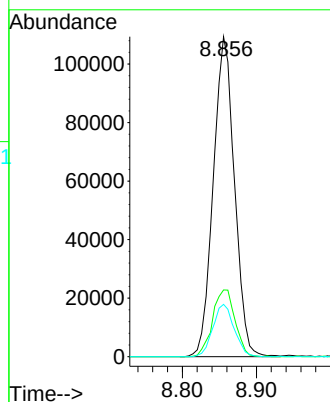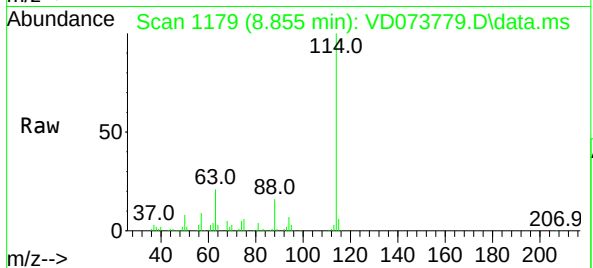

#35

Dibromofluoromethane

Concen: 55.913 ug/l

RT: 7.908 min Scan# 1018

Delta R.T. -0.000 min

Lab File: VD073779.D

Acq: 05 Jul 2022 17:35




Tgt Ion:113 Resp: 66018


Ion Ratio Lower Upper

113 100

111 105.0 81.8 122.6

192 16.2 14.8 22.2


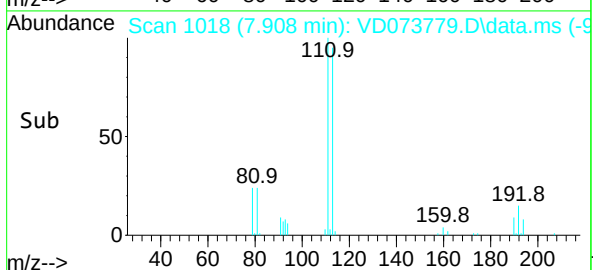
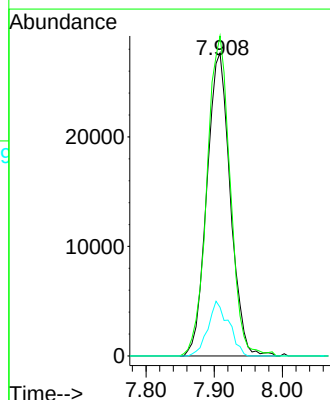
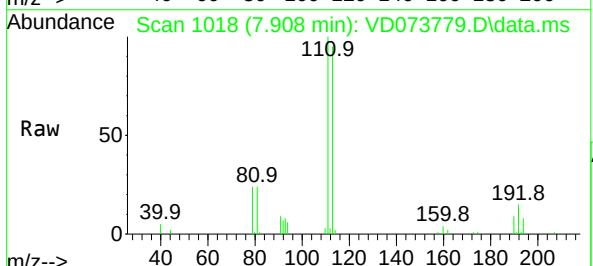


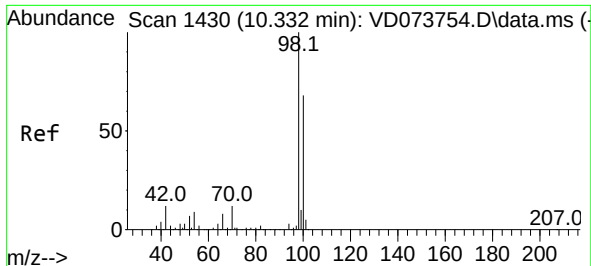

#50
Toluene-d8
Concen: 38.197 ug/l
RT: 10.332 min Scan# 1430
Delta R.T. -0.000 min
Lab File: VD073779.D
Acq: 05 Jul 2022 17:35




Instrument :
MSVOA_D
ClientSampleId :
SB-11ARE


Tgt Ion: 98 Resp: 165438
Ion Ratio Lower Upper
98 100
100 64.4 54.0 81.0

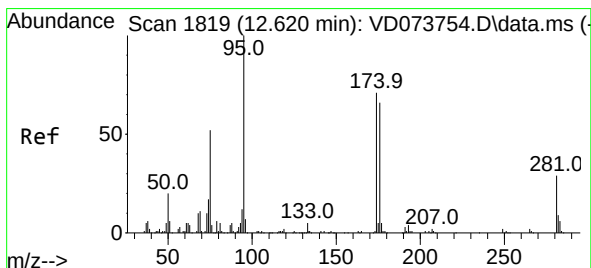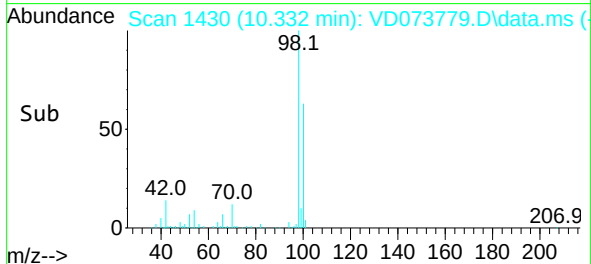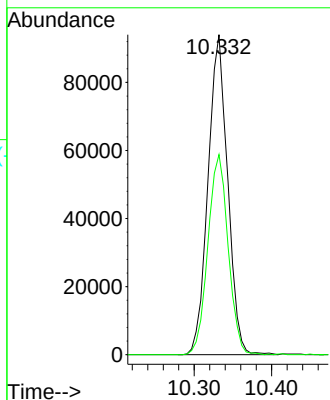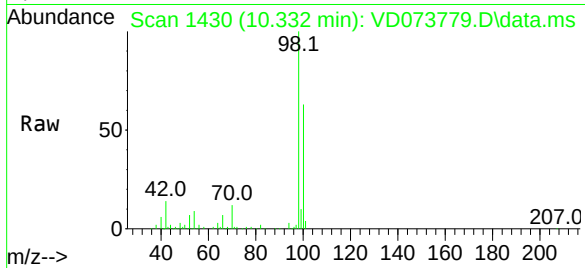

#62
4-Bromofluorobenzene
Concen: 30.139 ug/l
RT: 12.620 min Scan# 1819
Delta R.T. 0.000 min
Lab File: VD073779.D
Acq: 05 Jul 2022 17:35

Tgt Ion: 95 Resp: 51487
Ion Ratio Lower Upper
95 100
174 68.9 0.0 158.4
176 65.2 0.0 154.8

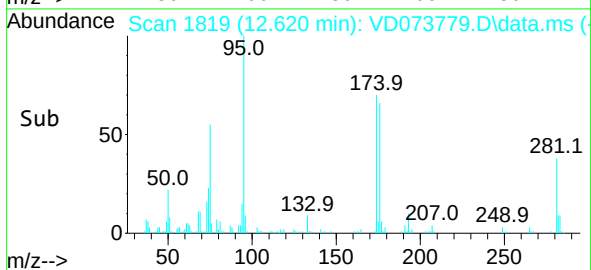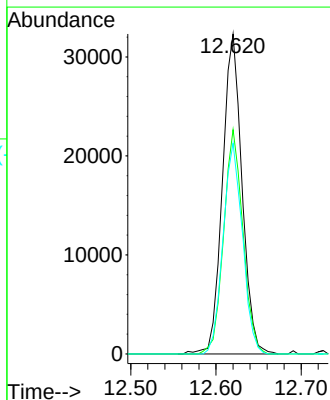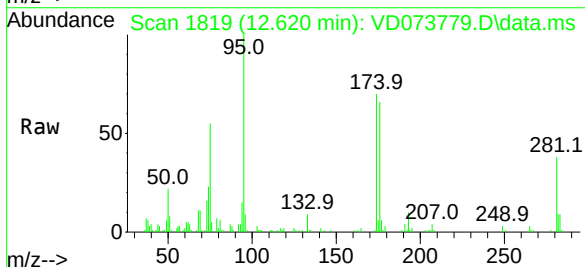

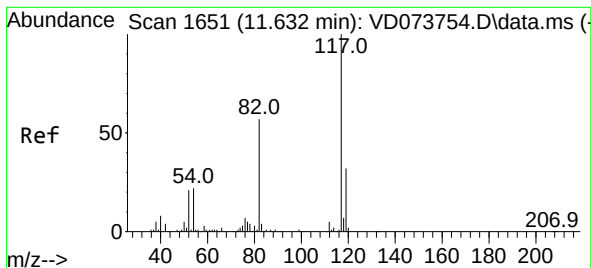

#63

Chlorobenzene-d5

Concen: 50.000 ug/l

RT: 11.632 min Scan# 1

Delta R.T. -0.000 min

Lab File: VD073779.D

Acq: 05 Jul 2022 17:35

Instrument :

MSVOA_D

ClientSampleId :

SB-11ARE





Tgt Ion:117 Resp: 152265

Ion Ratio Lower Upper

117 100

82 57.9 41.5 62.3

119 29.4 27.1 40.7

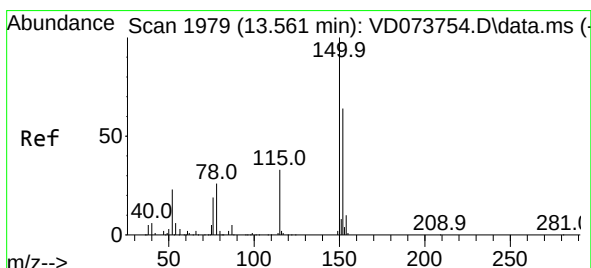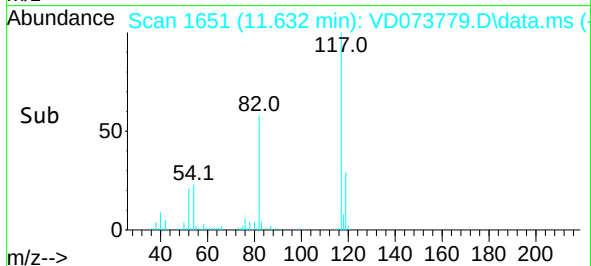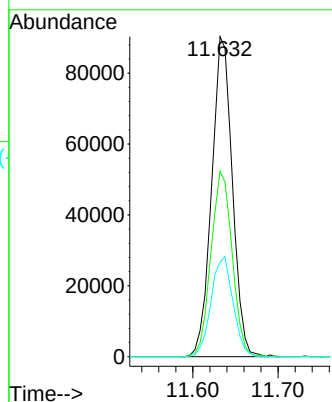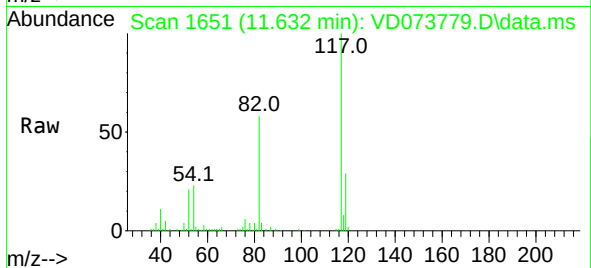

#72

1,4-Dichlorobenzene-d4

Concen: 50.000 ug/l

RT: 13.561 min Scan# 1979

Delta R.T. -0.000 min

Lab File: VD073779.D

Acq: 05 Jul 2022 17:35

Tgt Ion:152 Resp: 36997

Ion Ratio Lower Upper

152 100

115 66.4 30.6 91.6

150 156.5 0.0 355.0

