
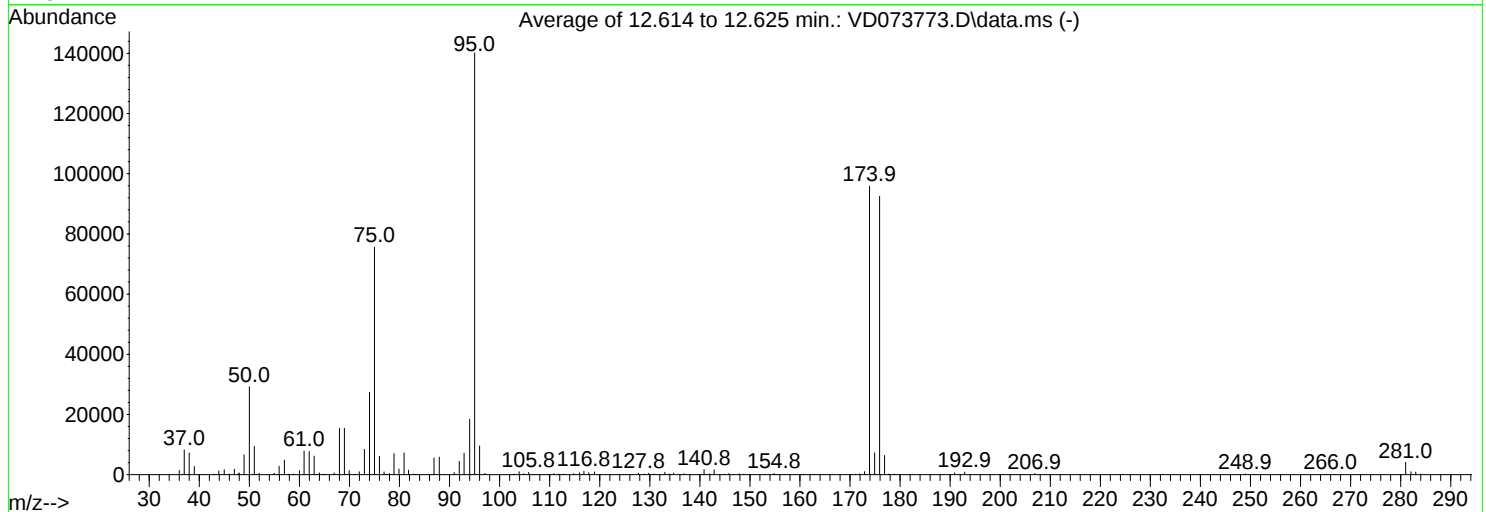


Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD070522\
Data File : VD073773.D
Acq On : 05 Jul 2022 13:36
Operator : VA/SY
Sample : BFB
Misc : 5.00G/5.00ml/MSVOA_D/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D063022S.M
Title : SW846 8260
Last Update : Tue Jul 05 10:05:34 2022

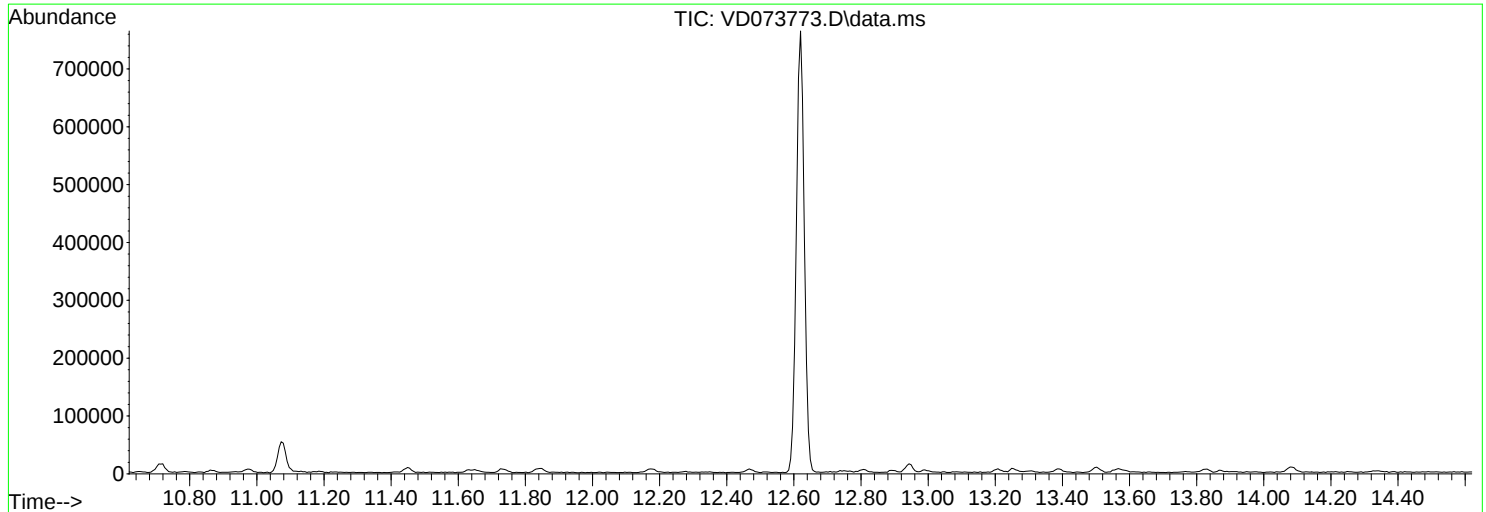

AutoFind: Scans 1818, 1819, 1820; Background Corrected with Scan 1810

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.9	29235	PASS
75	95	30	60	53.9	75613	PASS
95	95	100	100	100.0	140181	PASS
96	95	5	9	6.8	9496	PASS
173	174	0.00	2	1.1	1017	PASS
174	95	50	100	68.4	95877	PASS
175	174	5	9	7.5	7235	PASS
176	174	95	101	96.5	92491	PASS
177	176	5	9	6.9	6398	PASS