
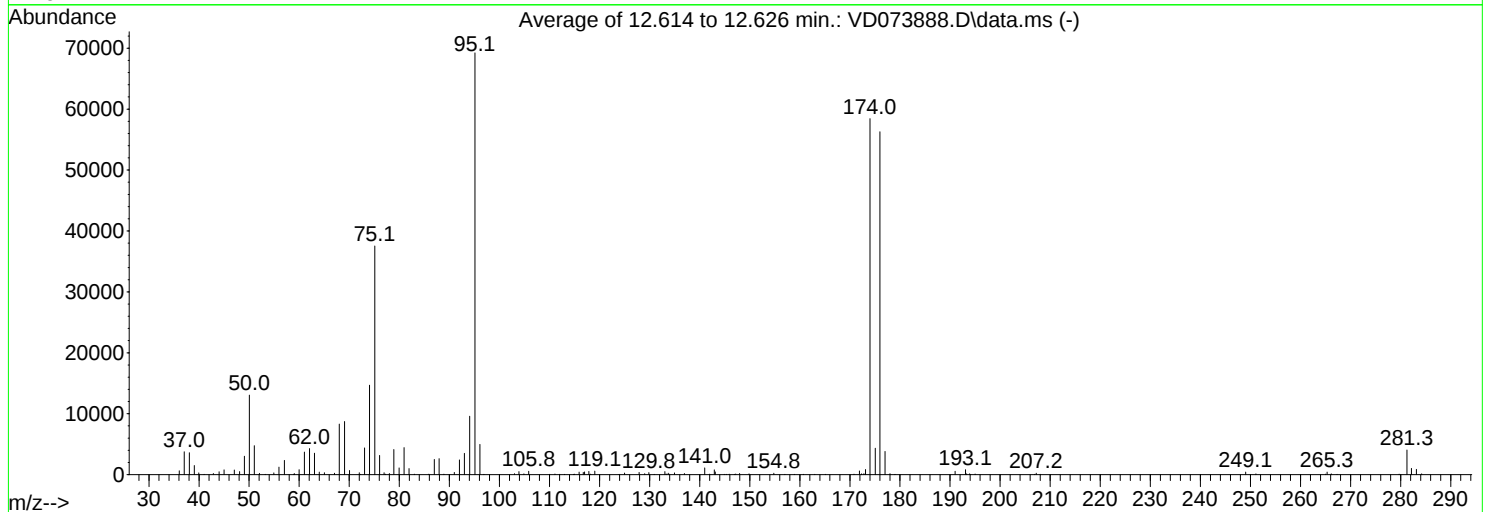


Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD072122\
Data File : VD073888.D
Acq On : 21 Jul 2022 09:42
Operator : VA/SY
Sample : BFB
Misc : 5.00G/5.00ml/MSVOA_D/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D071822S.M
Title : SW846 8260
Last Update : Wed Jul 20 15:29:08 2022

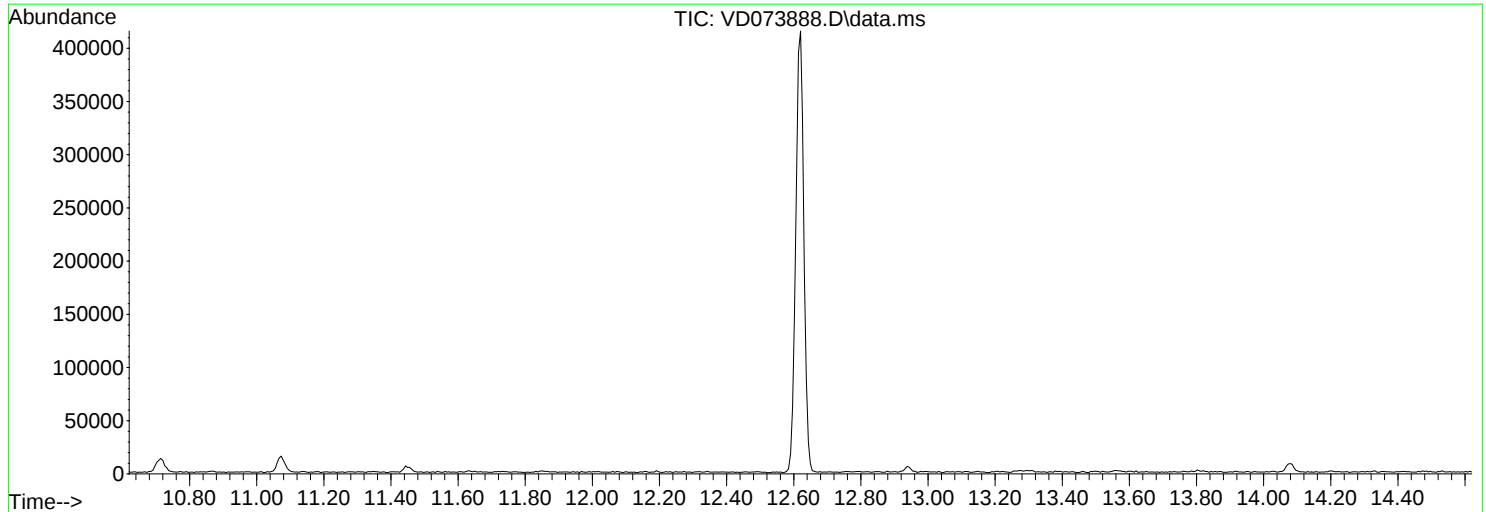

AutoFind: Scans 1818, 1819, 1820; Background Corrected with Scan 1809

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	18.9	13060	PASS
75	95	30	60	54.2	37539	PASS
95	95	100	100	100.0	69240	PASS
96	95	5	9	7.2	4962	PASS
173	174	0.00	2	1.4	843	PASS
174	95	50	100	84.4	58443	PASS
175	174	5	9	7.4	4340	PASS
176	174	95	101	96.3	56299	PASS
177	176	5	9	6.8	3802	PASS