

Data Path : Z:\VOASRV\HPCHEM1\MSVOA D\DATA\VD080620\
 Data File : VD066143.D
 Acq On : 06 Aug 2020 19:12
 Operator : VA/SY
 Sample : L3573-02
 Misc : 7.49G/5.00ml/MSVOA D/SOIL
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_D
 ClientSampleId :
 FK-GF-03-016-A

Quant Time: Aug 07 02:37:51 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_D\METHOD\82D080520S.M
 Quant Title : SW846 8260
 QLast Update : Wed Aug 05 13:49:25 2020
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	7.98	168	302925	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	8.86	114	534633	50.00	ug/l	0.00
63) Chlorobenzene-d5	11.64	117	589152	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.58	152	304878	50.00	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.33	65	140226	51.89	ug/l	0.00
Spiked Amount 50.000			Recovery	=	103.78%	
35) Dibromofluoromethane	7.91	113	167756	49.53	ug/l	0.00
Spiked Amount 50.000			Recovery	=	99.06%	
50) Toluene-d8	10.34	98	667516	53.41	ug/l	0.00
Spiked Amount 50.000			Recovery	=	106.82%	
62) 4-Bromofluorobenzene	12.64	95	280237	62.20	ug/l	0.00
Spiked Amount 50.000			Recovery	=	124.40%	
Target Compounds						
16) Acetone	4.16	43	4653	9.074	ug/l #	85


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA D\DATA\VD080620\
Data File : VD066143.D
Acq On : 06 Aug 2020 19:12
Operator : VA/SY
Sample : L3573-02
Misc : 7.49G/5.00ml/MSVOA D/SOIL
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
FK-GF-03-016-A

Quant Time: Aug 07 02:37:51 2020
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_D\METHOD\82D080520S.M
Quant Title : SW846 8260
QLast Update : Wed Aug 05 13:49:25 2020
Response via : Initial Calibration

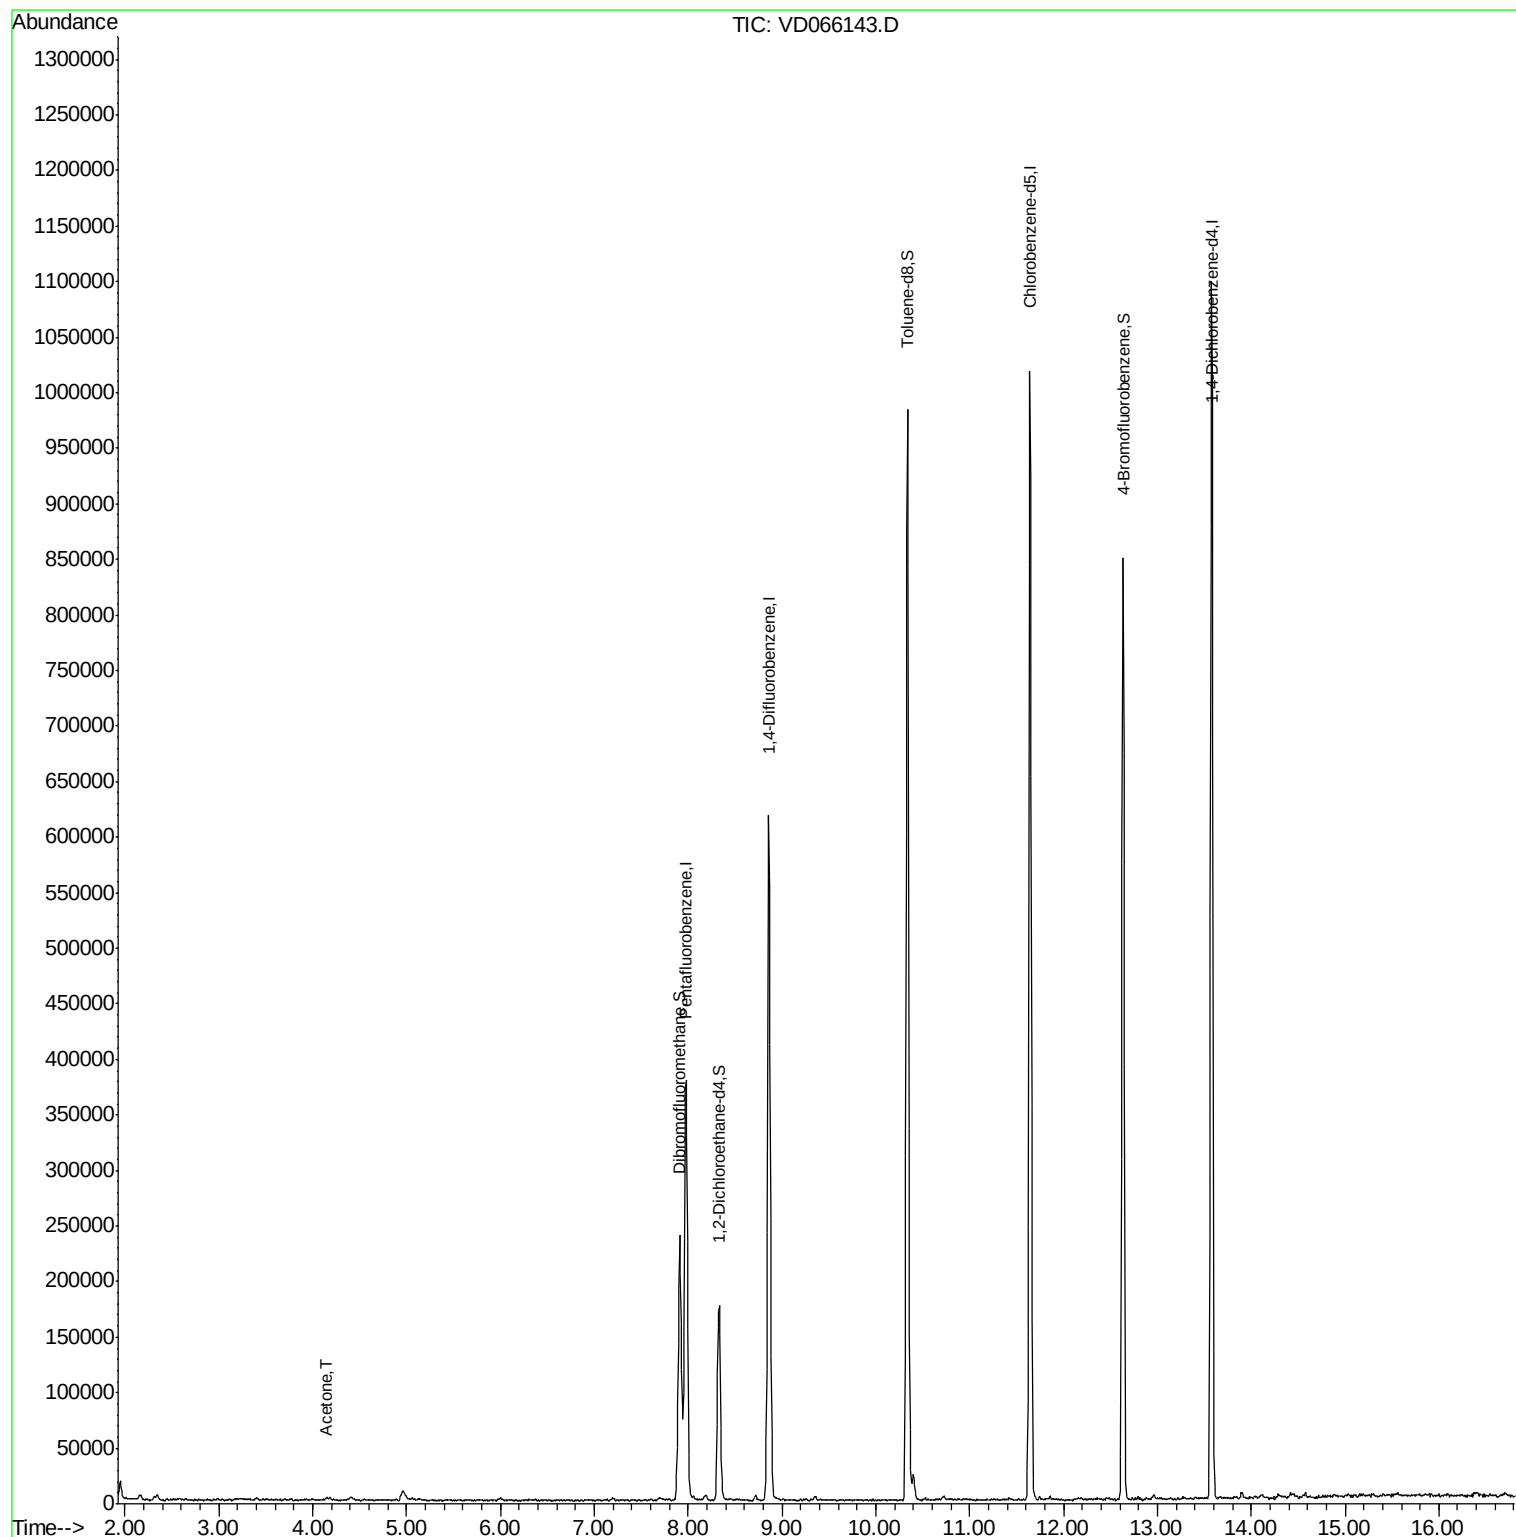

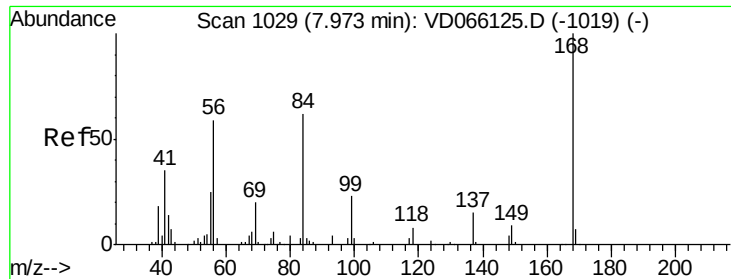

#1

Pentafluorobenzene

Concen: 50.000 ug/l

RT: 7.98 min Scan# 1030

Delta R.T. 0.01 min

Lab File: VD066143.D

Acq: 06 Aug 2020 19:12

Instrument :

MSVOA_D

ClientSampleId :


FK-GF-03-016-A

Tot Ion:168 Resp: 302925

Ion Ratio Lower Upper

168 100

99 52.7 42.2 63.4

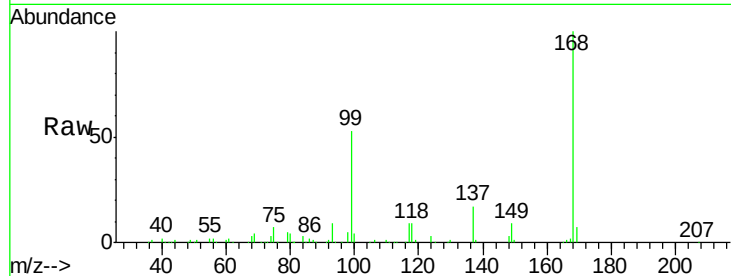

Abundance Ion 167.90 (167.60 to 168.60): V

Ion 98.90 (98.60 to 99.60): VDC

7.98



150000

100000

50000

0

Time-->

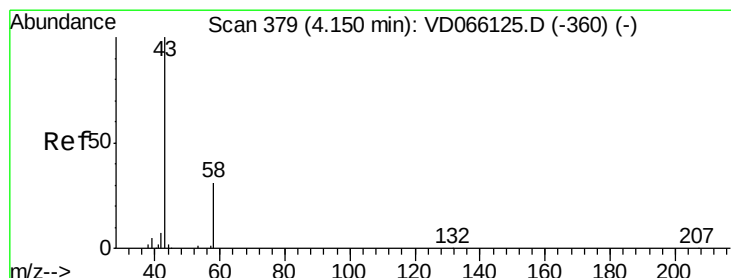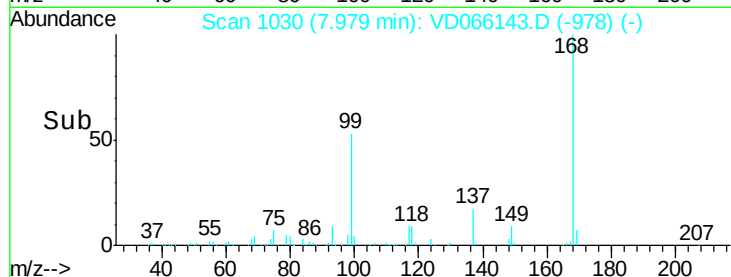

#16

Acetone

Concen: 9.074 ug/l

RT: 4.16 min Scan# 380

Delta R.T. 0.01 min

Lab File: VD066143.D


Acq: 06 Aug 2020 19:12

Tgt Ion: 43 Resp: 4653

Ion Ratio Lower Upper

43 100

58 39.3 24.7 37.1#

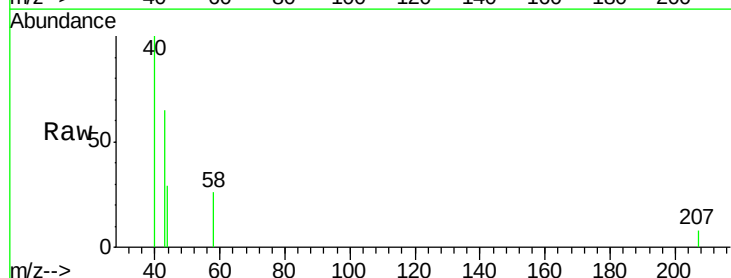

Abundance Ion 43.00 (42.70 to 43.70): VDC

Ion 58.00 (57.70 to 58.70): VDC

4.16


1500


1000

500

0

Time-->




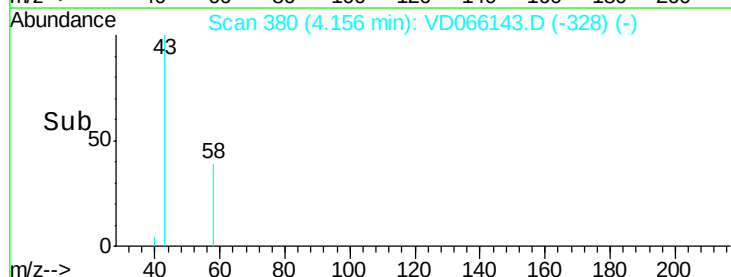


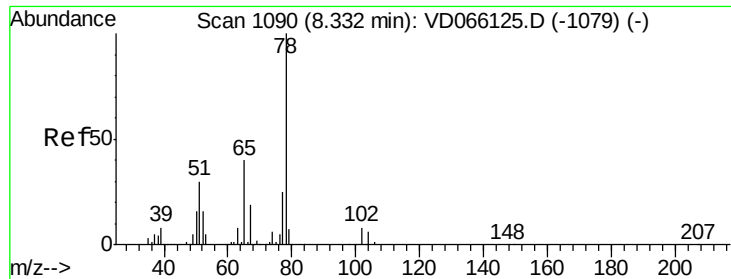

#33
 1,2-Dichloroethane-d4
 Concen: 51.887 ug/l
 RT: 8.33 min Scan# 1090
 Delta R.T. 0.00 min
 Lab File: VD066143.D
 Acq: 06 Aug 2020 19:12




Instrument :
 MSVOA_D
 ClientSampleId :
 FK-GF-03-016-A


Tot Ion: 65 Resp: 140226
 Ion Ratio Lower Upper
 65 100
 67 52.5 0.0 104.6

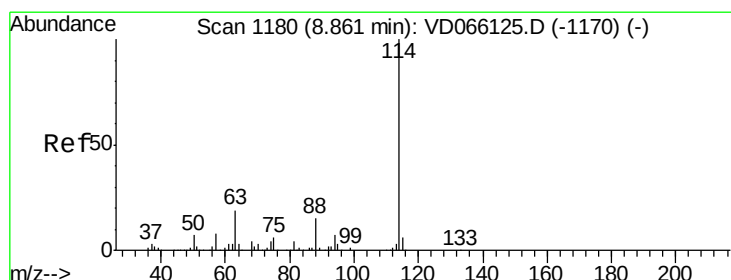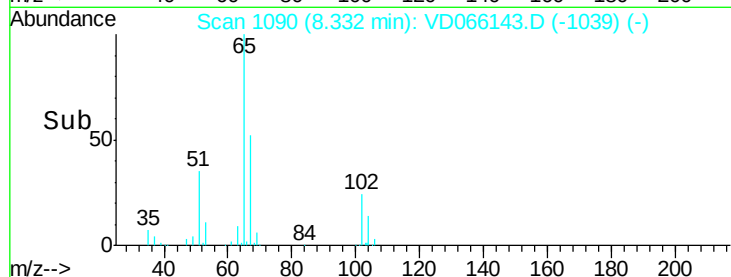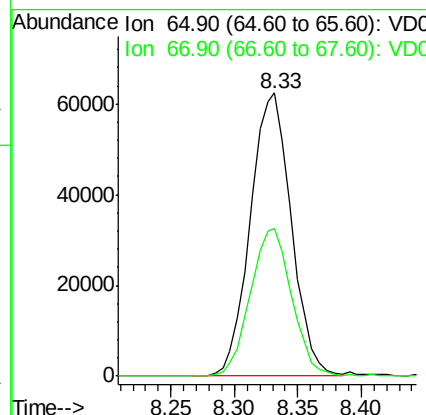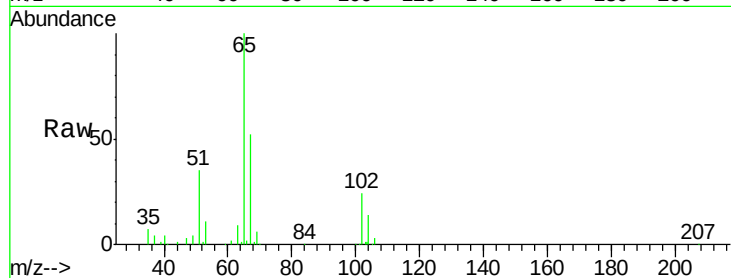

#34
 1,4-Difluorobenzene
 Concen: 50.000 ug/l
 RT: 8.86 min Scan# 1180
 Delta R.T. 0.00 min
 Lab File: VD066143.D
 Acq: 06 Aug 2020 19:12

Tgt Ion: 114 Resp: 534633
 Ion Ratio Lower Upper
 114 100
 63 18.7 0.0 38.6
 88 15.3 0.0 30.0


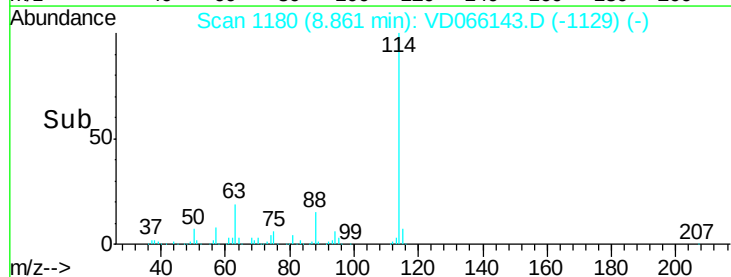
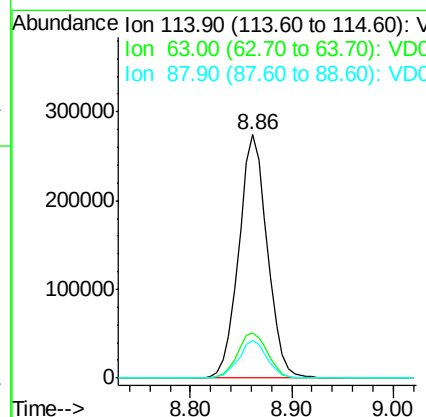
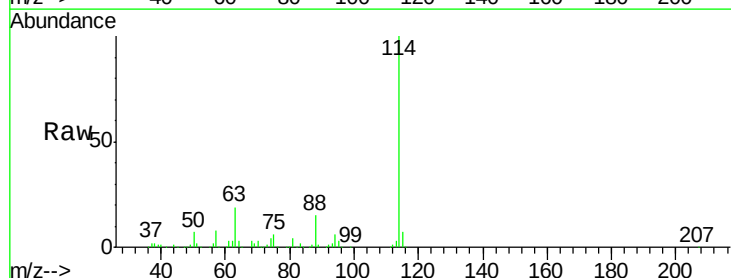


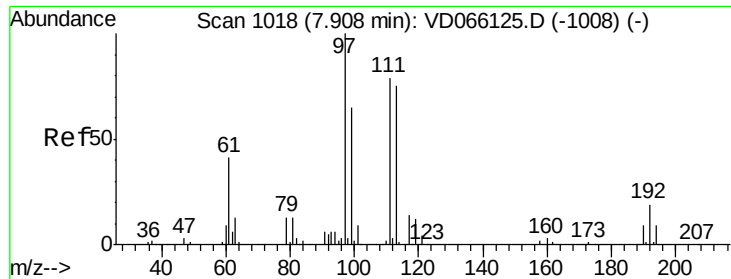

#35
 Dibromofluoromethane
 Concen: 49.532 ug/l
 RT: 7.91 min Scan# 1019
 Delta R.T. 0.01 min
 Lab File: VD066143.D
 Acq: 06 Aug 2020 19:12




Instrument :
 MSVOA_D
 ClientSampleId :
 FK-GF-03-016-A


Tot Ion	Ratio	Lower	Upper
113	100		
111	101.6	80.7	121.1
192	21.4	18.4	27.6

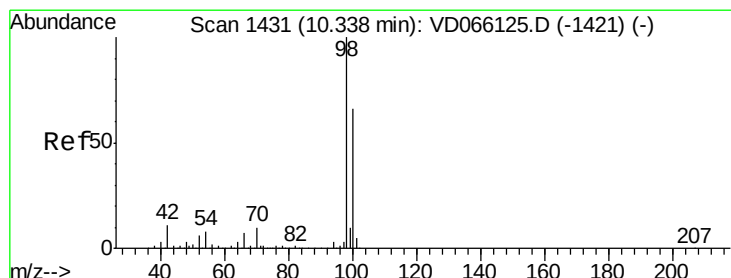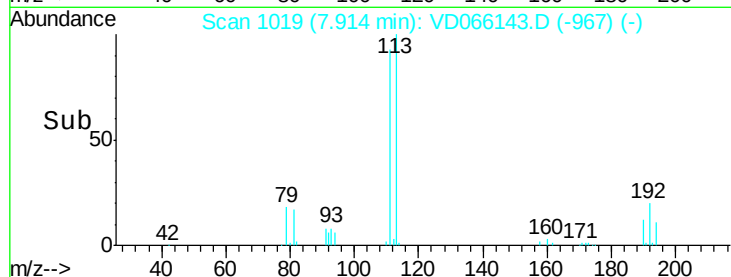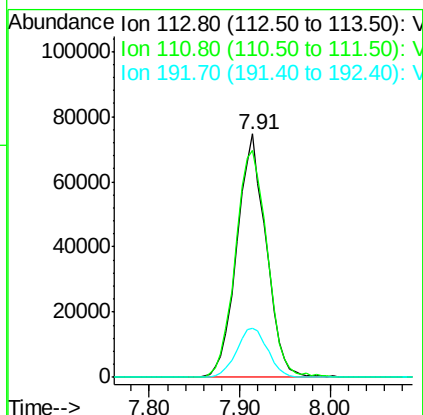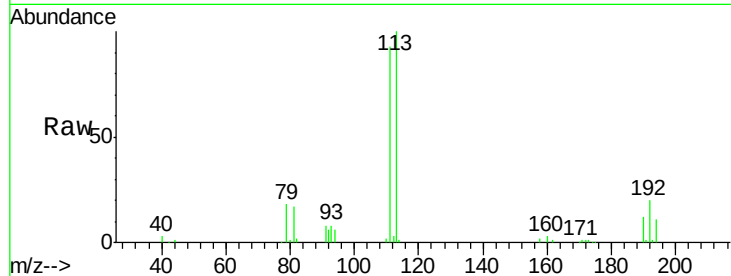

#50
 Toluene-d8
 Concen: 53.409 ug/l
 RT: 10.34 min Scan# 1431
 Delta R.T. 0.00 min
 Lab File: VD066143.D
 Acq: 06 Aug 2020 19:12

Tgt Ion	Ratio	Lower	Upper
98	100		
100	65.0	52.6	78.8

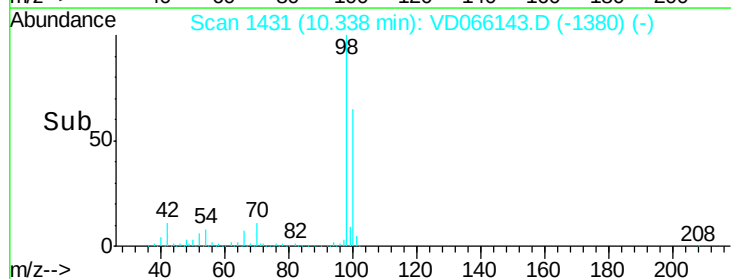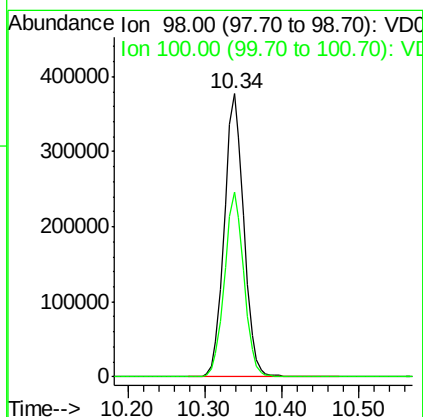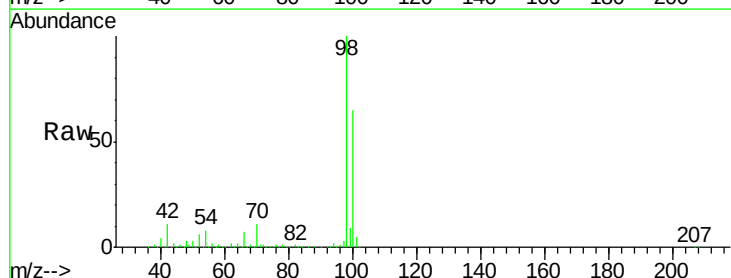

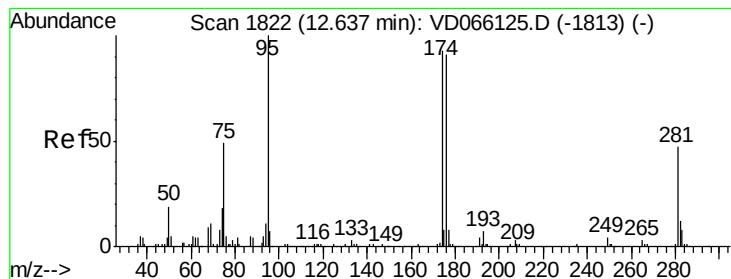

#62

4-Bromofluorobenzene

Concen: 62.204 ug/l

RT: 12.64 min Scan# 1822

Delta R.T. 0.00 min

Lab File: VD066143.D

Acq: 06 Aug 2020 19:12

Instrument :

MSVOA_D

ClientSampleId :

FK-GF-03-016-A


Tot Ion: 95 Resp: 280237

Ion Ratio Lower Upper

95 100

174 88.8 0.0 180.8




176 86.0 0.0 181.2

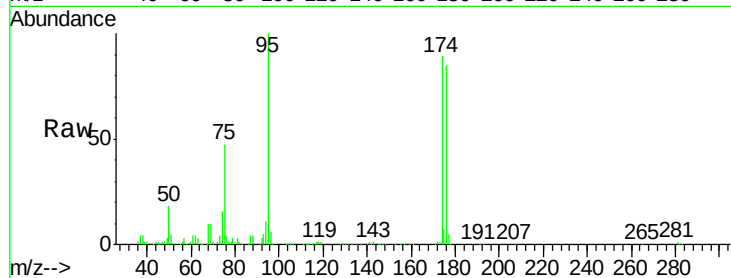

Abundance Ion 94.90 (94.60 to 95.60): V

Ion 173.80 (173.50 to 174.50): V

Ion 175.80 (175.50 to 176.50): V

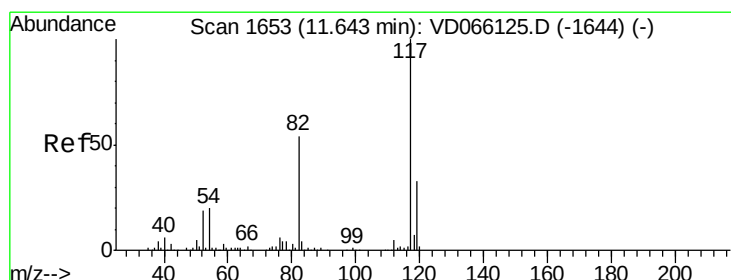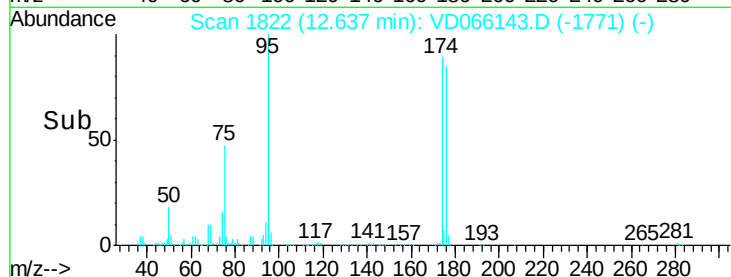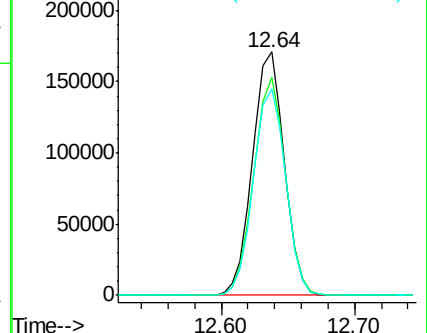

#63

Chlorobenzene-d5

Concen: 50.000 ug/l

RT: 11.64 min Scan# 1653

Delta R.T. 0.00 min

Lab File: VD066143.D

Acq: 06 Aug 2020 19:12


Tgt Ion: 117 Resp: 589152

Ion Ratio Lower Upper

117 100

82 54.1 43.0 64.4



119 32.8 26.1 39.1

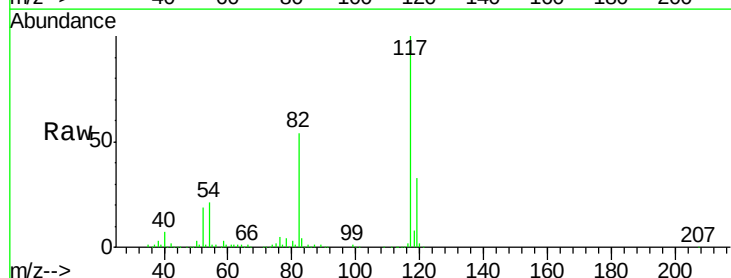


Abundance Ion 116.90 (116.60 to 117.60): V

Ion 82.00 (81.70 to 82.70): V

Ion 118.90 (118.60 to 119.60): V

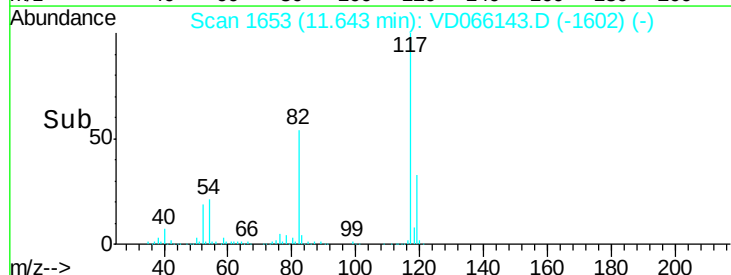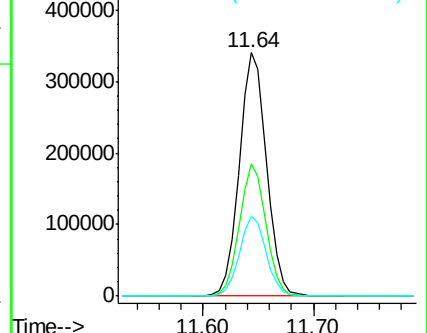

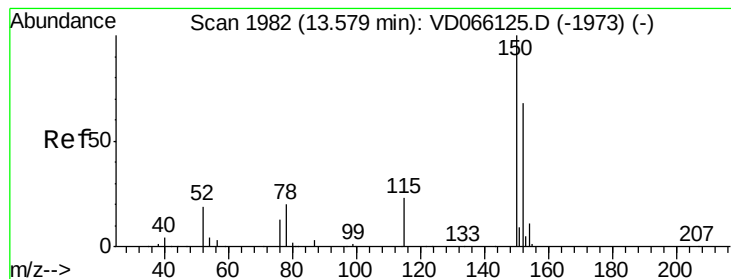

#72

1,4-Dichlorobenzene-d4

Concen: 50.000 ug/l

RT: 13.58 min Scan# 1982

Delta R.T. 0.00 min

Lab File: VD066143.D

Acq: 06 Aug 2020 19:12

Instrument :

MSVOA_D

ClientSampleId :

FK-GF-03-016-A


Tot Ion:152 Resp: 304878

Ion Ratio Lower Upper

152 100

115 54.8 28.0 83.9

150 156.2 0.0 346.4

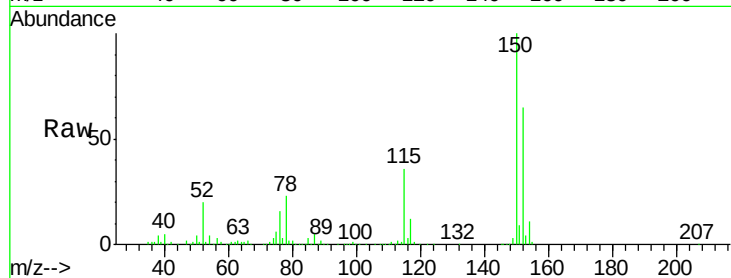

Abundance Ion 151.90 (151.60 to 152.60): V

Ion 114.90 (114.60 to 115.60): V

Ion 149.90 (149.60 to 150.60): V

