


Data Path : Z:\voasrv\HPCHEM1\MSVOA D\Data\VD081020\
Data File : VD066161.D
Acq On : 10 Aug 2020 13:06
Operator : VA/SY
Sample : BFB
Misc : 5.00G/5.00ml/MSVOA D/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_D\METHOD\82D080520S.M
Title : SW846 8260
Last Update : Wed Aug 05 13:49:25 2020

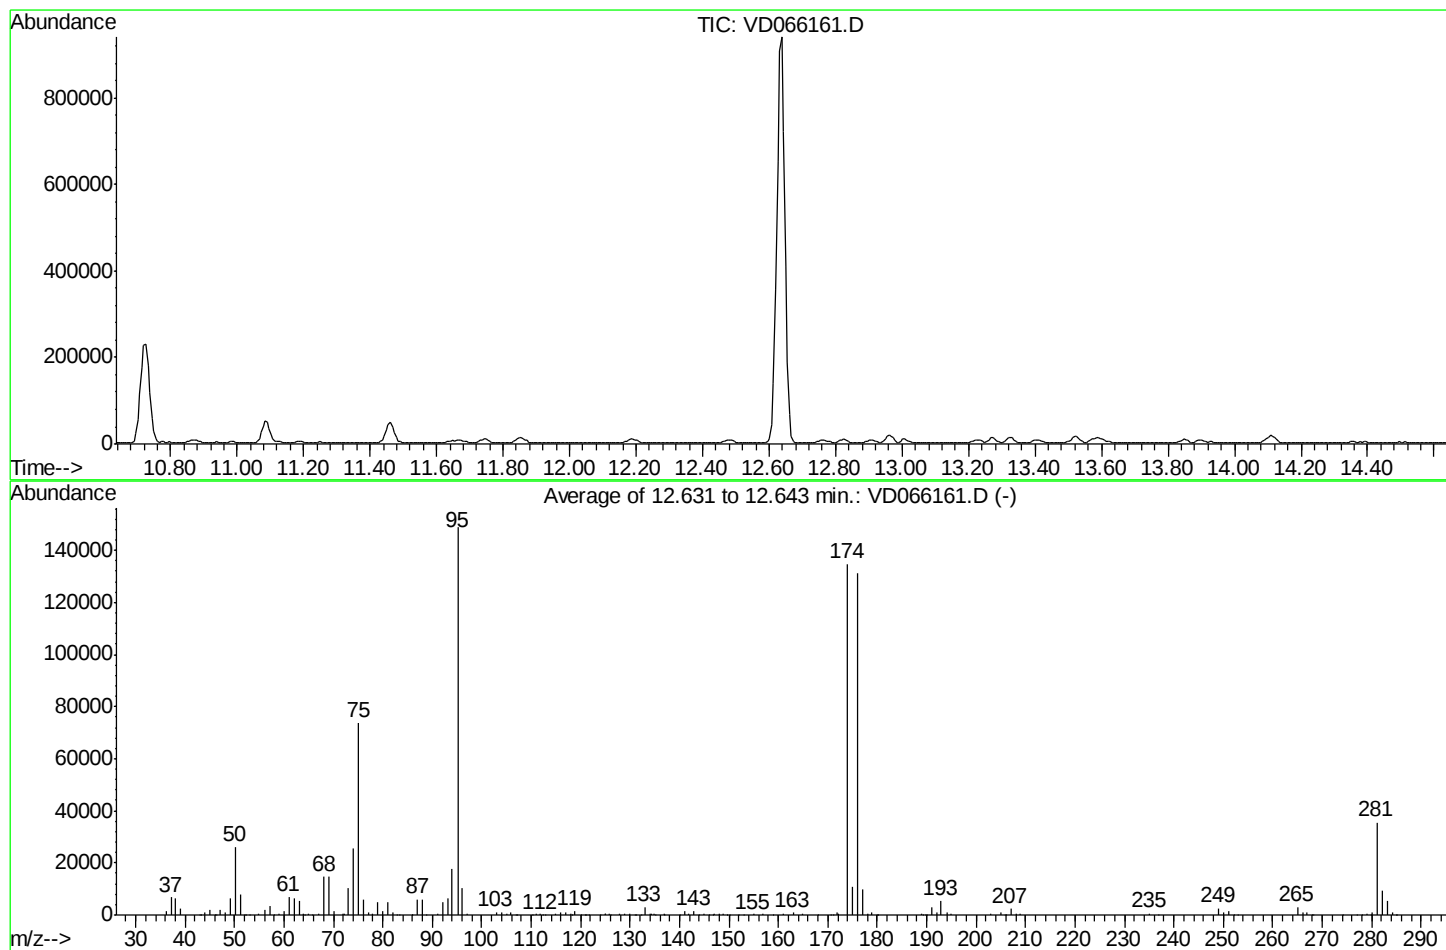

AutoFind: Scans 1821, 1822, 1823; Background Corrected with Scan 1811

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.6	26186	PASS
75	95	30	60	49.6	73834	PASS
95	95	100	100	100.0	148821	PASS
96	95	5	9	6.8	10187	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	100	90.6	134888	PASS
175	174	5	9	8.2	11029	PASS
176	174	95	101	97.3	131272	PASS
177	176	5	9	7.5	9793	PASS