


Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD081120\
 Data File : VD066178.D
 Acq On : 11 Aug 2020 09:34
 Operator : VA/SY
 Sample : BFB
 Misc : 5.00G/5.00ml/MSVOA_D/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_D
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_D\METHOD\82D080520S.M
 Title : SW846 8260
 Last Update : Wed Aug 05 13:49:25 2020

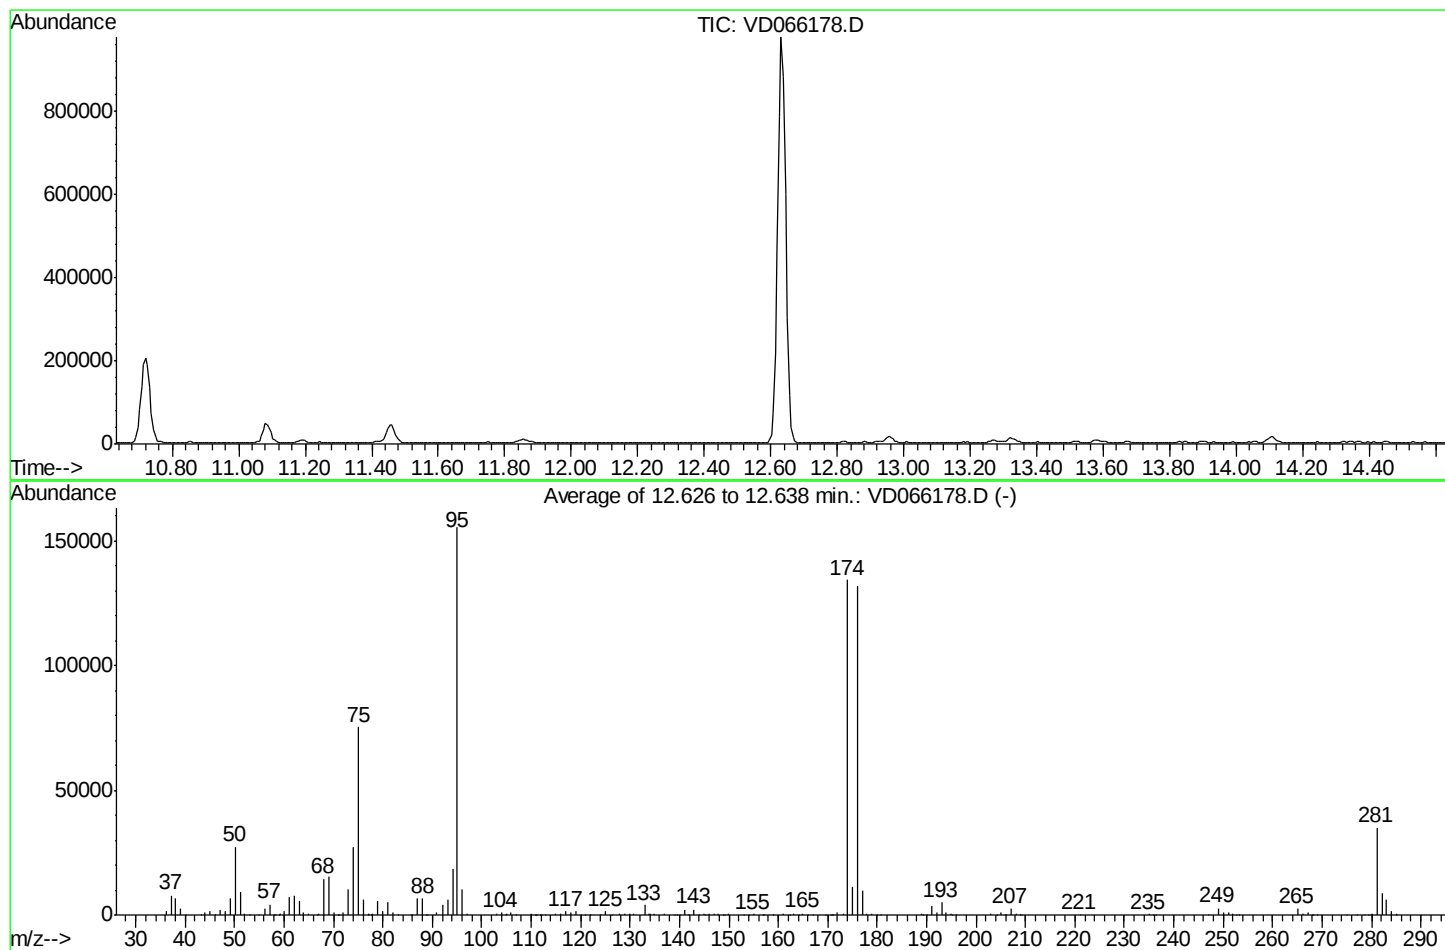

AutoFind: Scans 1820, 1821, 1822; Background Corrected with Scan 1812

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.6	27312	PASS
75	95	30	60	48.5	75400	PASS
95	95	100	100	100.0	155413	PASS
96	95	5	9	6.7	10470	PASS
173	174	0.00	2	0.5	732	PASS
174	95	50	100	86.5	134365	PASS
175	174	5	9	8.6	11529	PASS
176	174	95	101	98.3	132112	PASS
177	176	5	9	7.3	9597	PASS