


Data Path : Z:\voasrv\HPCHEM1\MSVOA D\Data\VD081319\
 Data File : VD063548.D
 Acq On : 14 Aug 2019 1:14
 Operator : JC/SY
 Sample : BFB
 Misc : 5.00µl/5ml/MSVOA D/SOIL
 ALS Vial : 37 Sample Multiplier: 1

Instrument :
 MSVOA_D
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_D\METHOD\82D080919S.M
 Title : SW846 8260
 Last Update : Sat Aug 10 06:42:47 2019

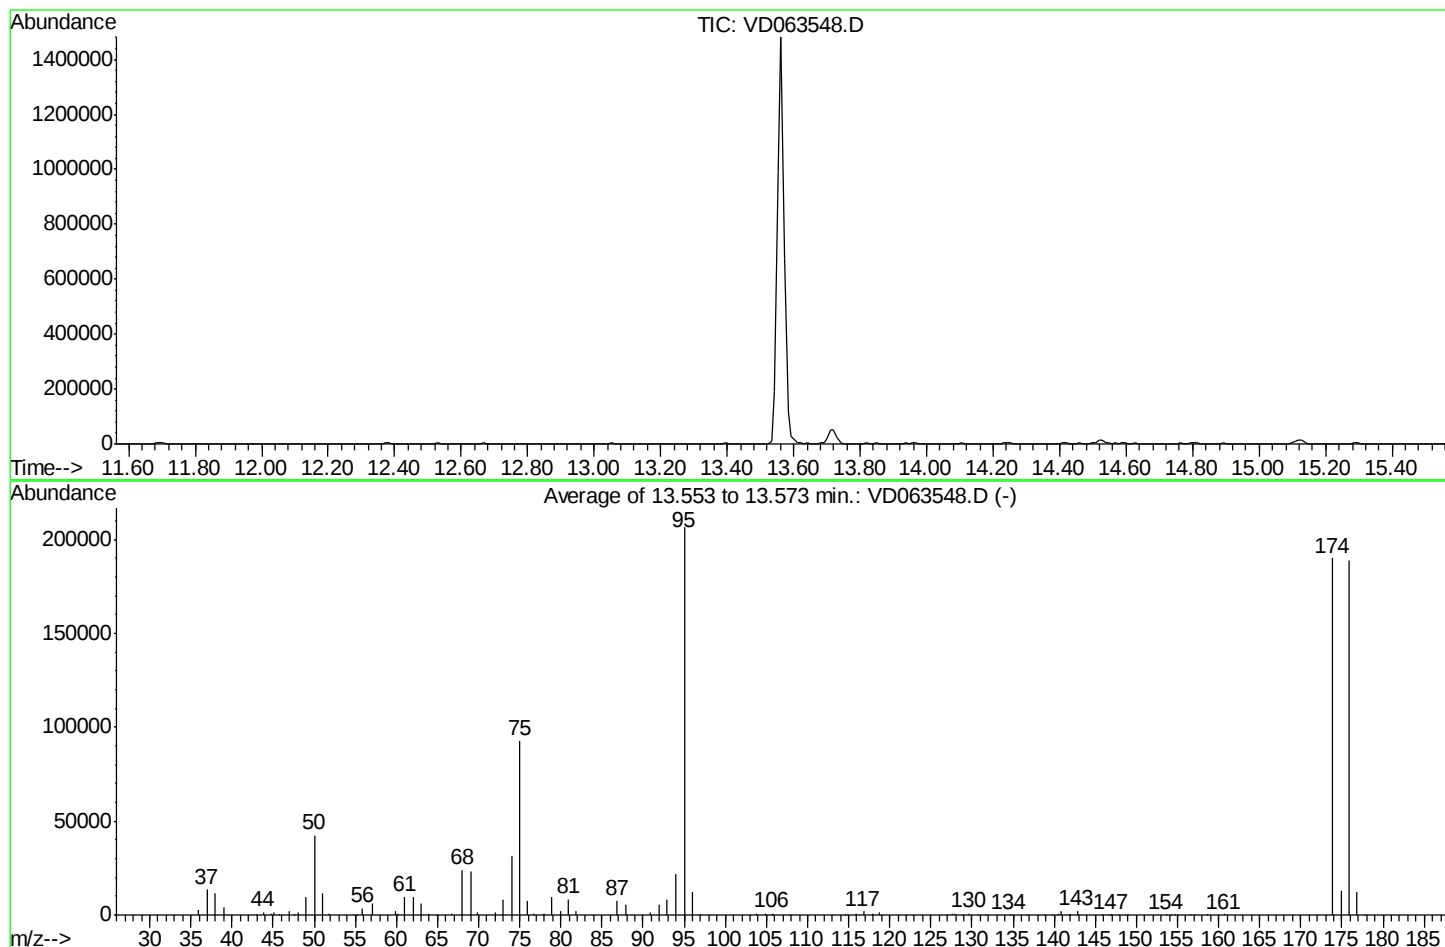

AutoFind: Scans 1232, 1233, 1234; Background Corrected with Scan 1227

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.5	42328	PASS
75	95	30	60	45.0	92797	PASS
95	95	100	100	100.0	206386	PASS
96	95	5	9	5.9	12262	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	100	92.1	190101	PASS
175	174	5	9	6.8	12972	PASS
176	174	95	101	99.1	188458	PASS
177	176	5	9	6.3	11967	PASS