


Data Path : Z:\voasrv\HPCHEM1\MSVOA D\Data\VD081320\
Data File : VD066208.D
Acq On : 13 Aug 2020 12:20
Operator : VA/SY
Sample : BFB
Misc : 5.00G/5.00ml/MSVOA D/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_D\METHOD\82D080520S.M
Title : SW846 8260
Last Update : Wed Aug 05 13:49:25 2020

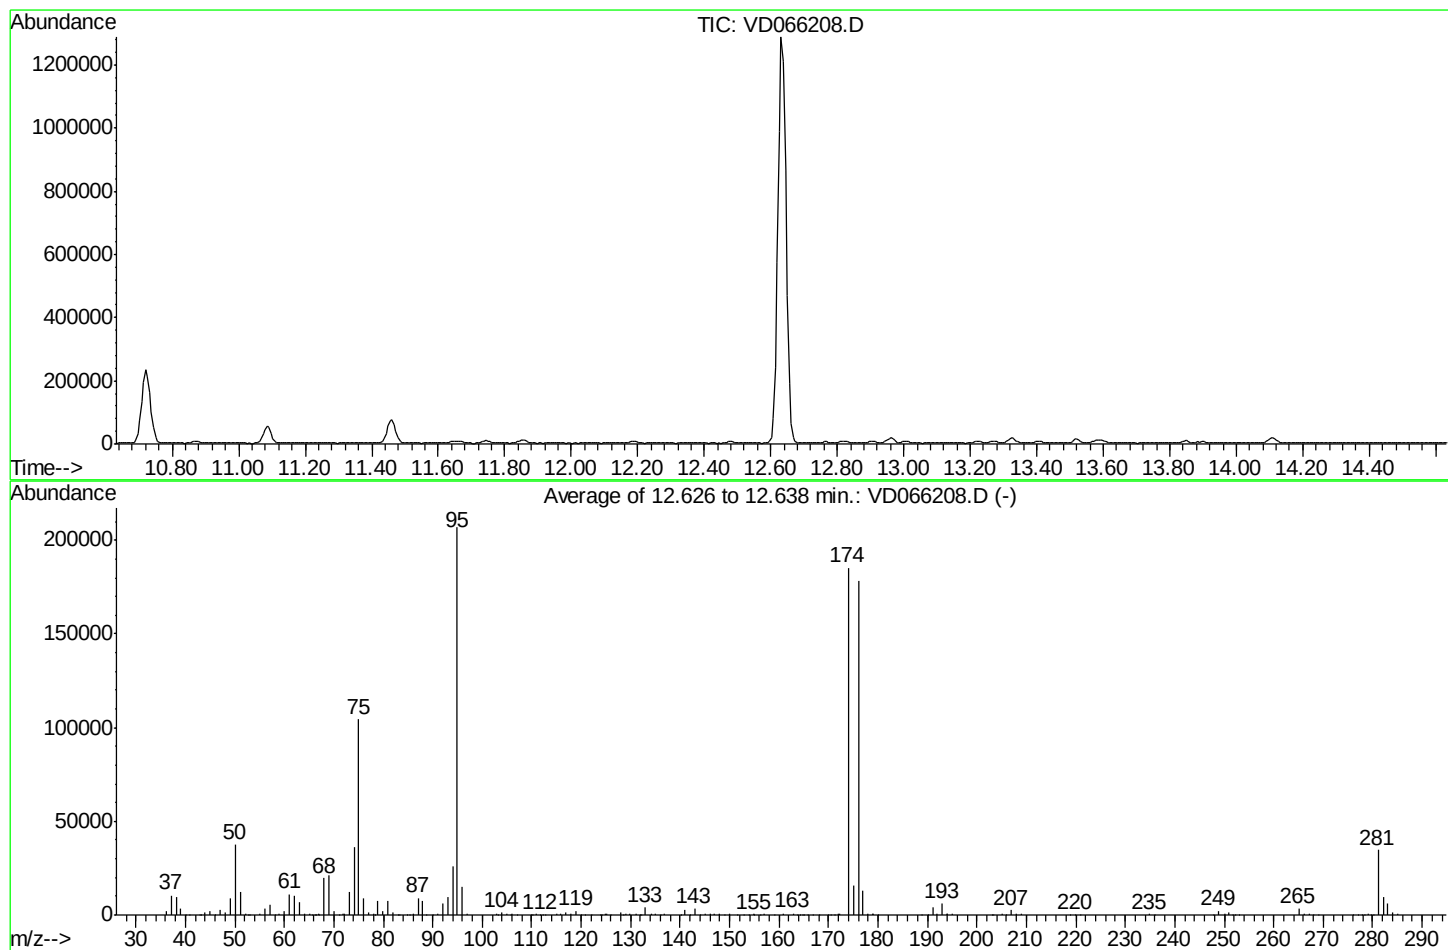

AutoFind: Scans 1820, 1821, 1822; Background Corrected with Scan 1811

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.1	37477	PASS
75	95	30	60	50.5	104440	PASS
95	95	100	100	100.0	206869	PASS
96	95	5	9	7.4	15359	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	100	89.6	185280	PASS
175	174	5	9	8.4	15634	PASS
176	174	95	101	96.4	178624	PASS
177	176	5	9	7.1	12719	PASS