

Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD081621\
 Data File : VD070072.D
 Acq On : 16 Aug 2021 17:46
 Operator : VA/SY
 Sample : M3368-08
 Misc : 5.76G/5.00ml/MSVOA_D/SOIL
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_D
 ClientSampleId :
 SWCS-07-0002

Quant Time: Aug 17 03:57:16 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D081321S.M
 Quant Title : SW846 8260
 QLast Update : Sat Aug 14 02:33:51 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	7.979	168	518865	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	8.861	114	1081247	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.638	117	1016205	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.567	152	395752	50.000	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.326	65	367006	60.139	ug/l	0.00
Spiked Amount	50.000	Range	50 - 163	Recovery	=	120.280%
35) Dibromofluoromethane	7.914	113	360719	51.638	ug/l	0.00
Spiked Amount	50.000	Range	54 - 147	Recovery	=	103.280%
50) Toluene-d8	10.338	98	1392520	51.252	ug/l	0.00
Spiked Amount	50.000	Range	49 - 140	Recovery	=	102.500%
62) 4-Bromofluorobenzene	12.626	95	433833	48.478	ug/l	0.00
Spiked Amount	50.000	Range	25 - 144	Recovery	=	96.960%


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD081621\
Data File : VD070072.D
Acq On : 16 Aug 2021 17:46
Operator : VA/SY
Sample : M3368-08
Misc : 5.76G/5.00ml/MSVOA_D/SOIL
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
SWCS-07-0002

Quant Time: Aug 17 03:57:16 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D081321S.M
Quant Title : SW846 8260
QLast Update : Sat Aug 14 02:33:51 2021
Response via : Initial Calibration




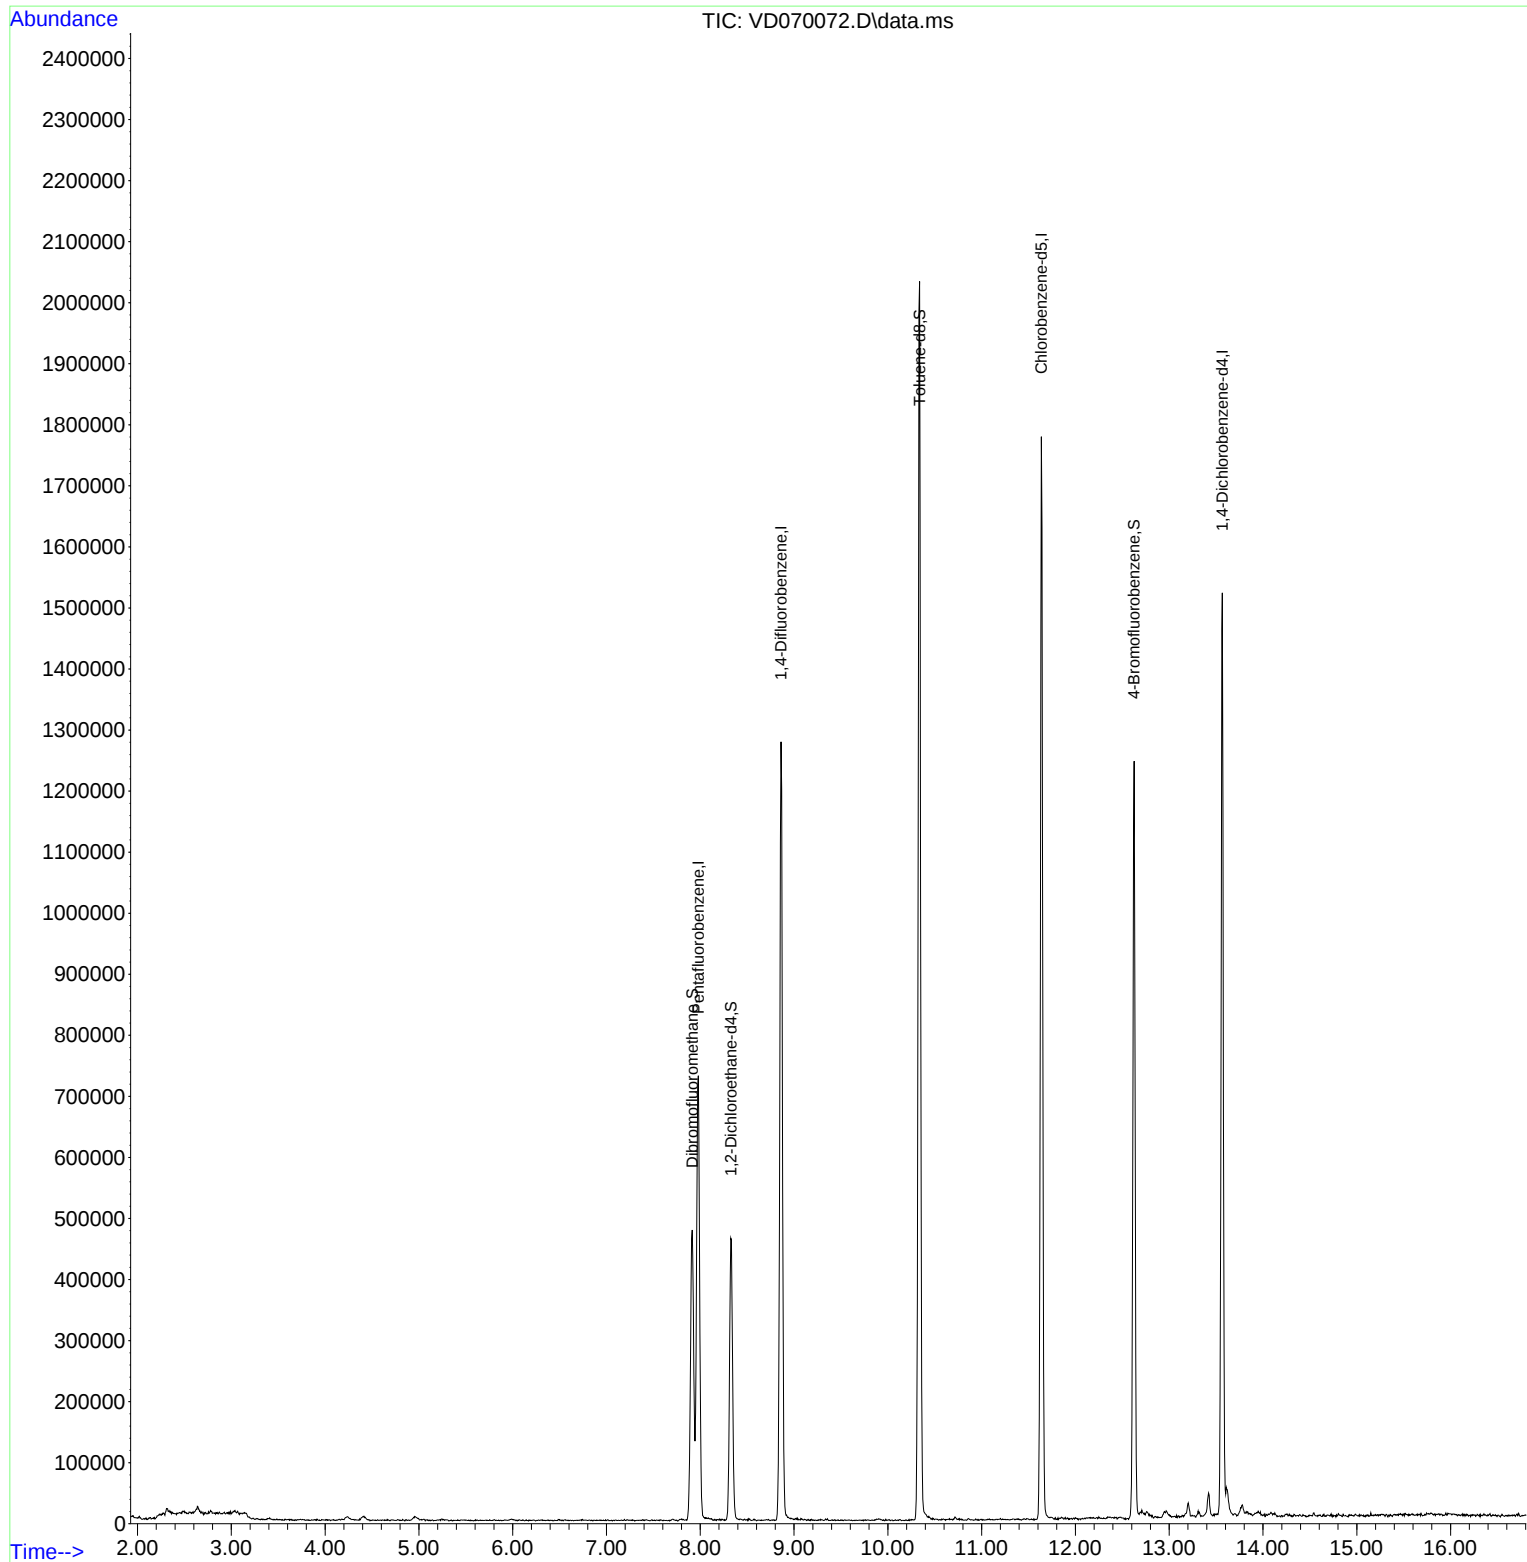


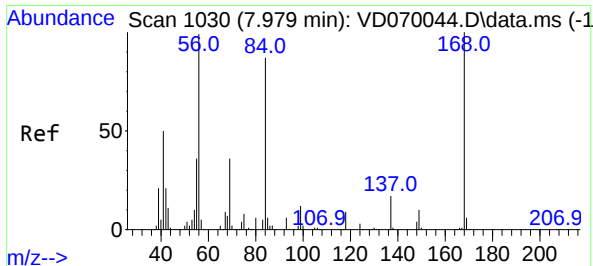

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 7.979 min Scan# 1030
Delta R.T. -0.000 min
Lab File: VD070072.D
Acq: 16 Aug 2021 17:46




Instrument :
MSVOA_D
ClientSampleId :
SWCS-07-0002


Tgt Ion:168 Resp: 518865
Ion Ratio Lower Upper
168 100
99 64.0 50.3 75.5

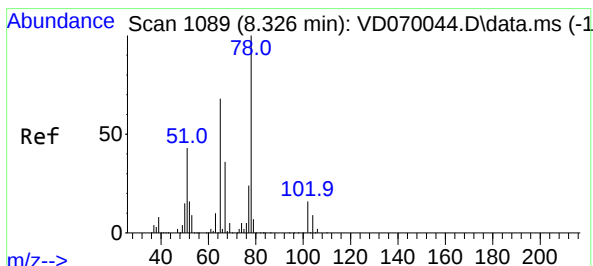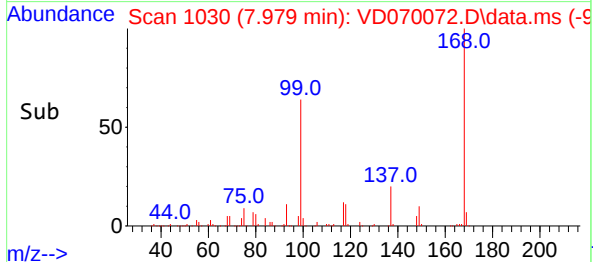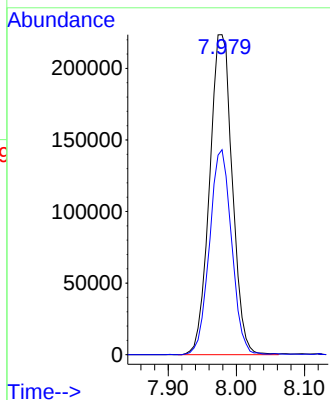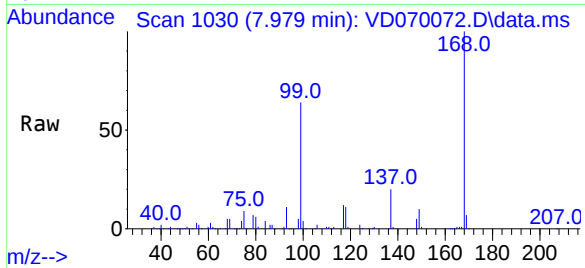

#33
1,2-Dichloroethane-d4
Concen: 60.139 ug/l
RT: 8.326 min Scan# 1089
Delta R.T. -0.000 min
Lab File: VD070072.D
Acq: 16 Aug 2021 17:46

Tgt Ion: 65 Resp: 367006
Ion Ratio Lower Upper
65 100
67 55.3 0.0 107.8


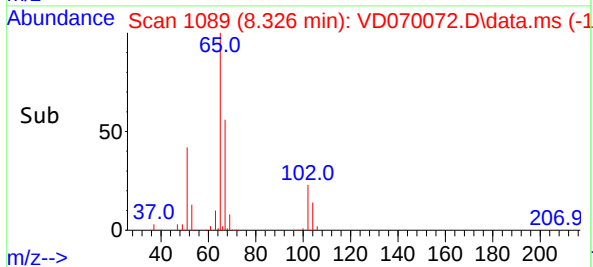
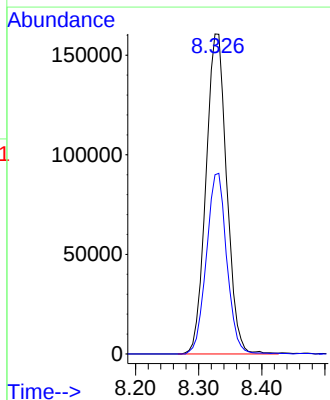
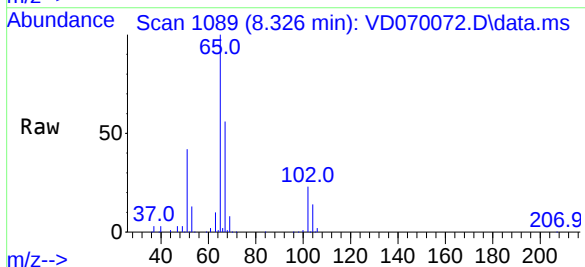


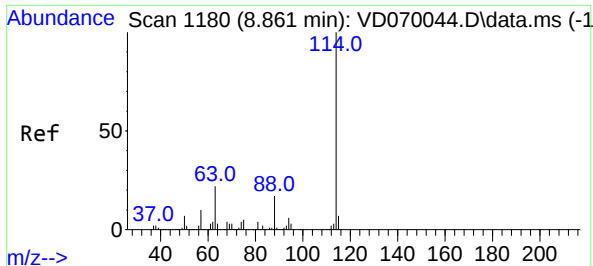

#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 8.861 min Scan# 1180
Delta R.T. -0.000 min
Lab File: VD070072.D
Acq: 16 Aug 2021 17:46




Instrument :
MSVOA_D
ClientSampleId :
SWCS-07-0002


Tgt Ion:114 Resp: 1081247
Ion Ratio Lower Upper
114 100
63 21.3 0.0 43.6
88 16.4 0.0 33.4

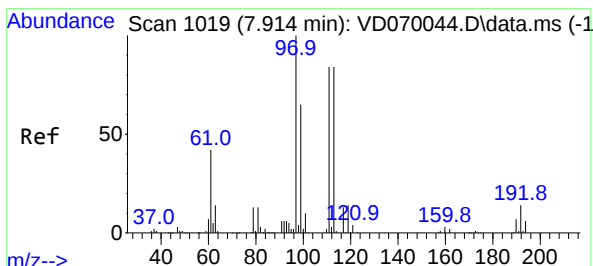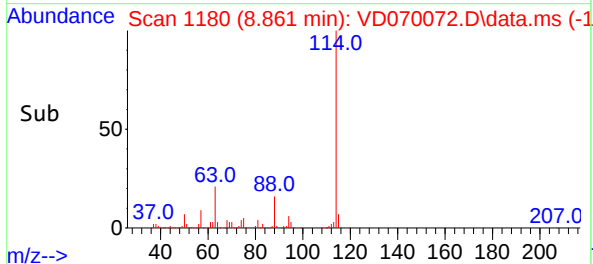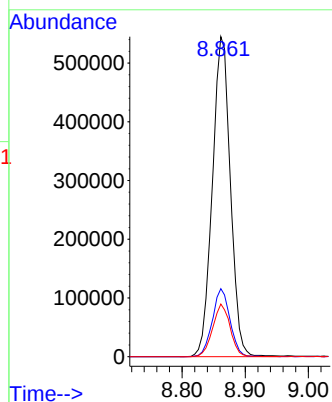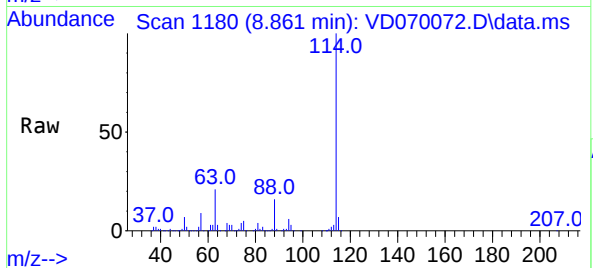

#35
Dibromofluoromethane
Concen: 51.638 ug/l
RT: 7.914 min Scan# 1019
Delta R.T. -0.000 min
Lab File: VD070072.D
Acq: 16 Aug 2021 17:46

Tgt Ion:113 Resp: 360719
Ion Ratio Lower Upper
113 100
111 102.5 81.8 122.6
192 16.3 13.2 19.8


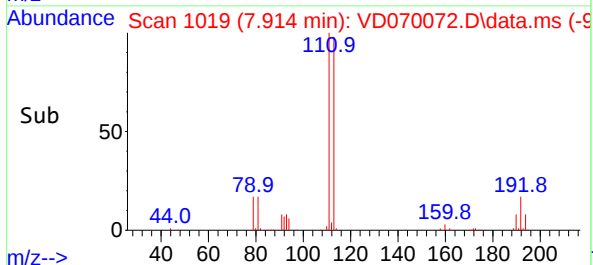
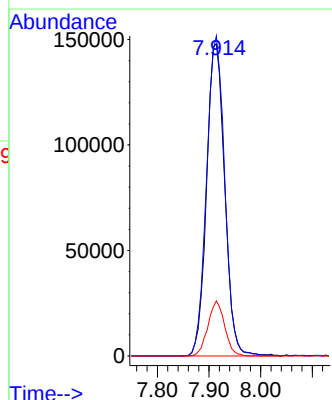
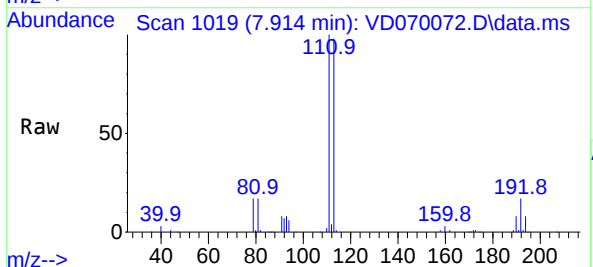


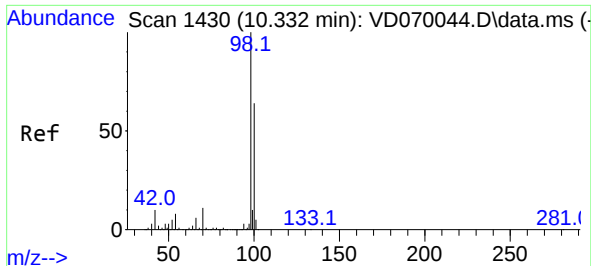

#50
Toluene-d8
Concen: 51.252 ug/l
RT: 10.338 min Scan# 1431
Delta R.T. 0.006 min
Lab File: VD070072.D
Acq: 16 Aug 2021 17:46




Instrument :
MSVOA_D
ClientSampleId :
SWCS-07-0002


Tgt Ion: 98 Resp: 1392520
Ion Ratio Lower Upper
98 100
100 64.2 52.6 78.8

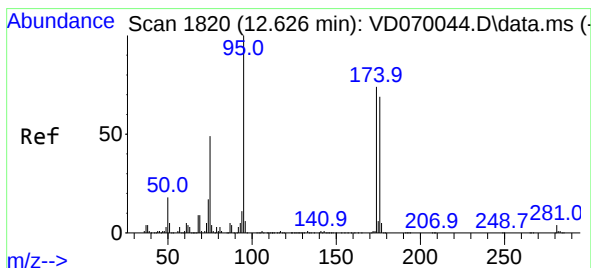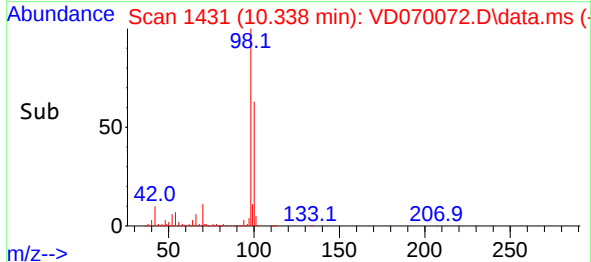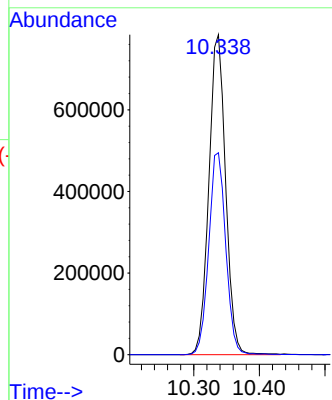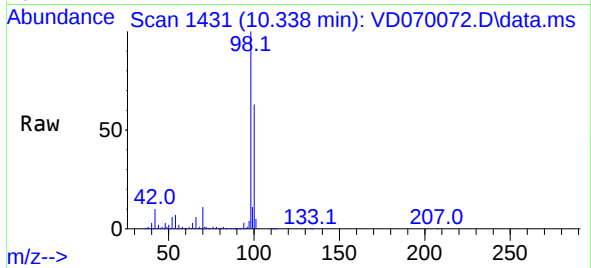

#62
4-Bromofluorobenzene
Concen: 48.478 ug/l
RT: 12.626 min Scan# 1820
Delta R.T. -0.000 min
Lab File: VD070072.D
Acq: 16 Aug 2021 17:46

Tgt Ion: 95 Resp: 433833
Ion Ratio Lower Upper
95 100
174 70.8 0.0 141.6
176 68.0 0.0 138.2


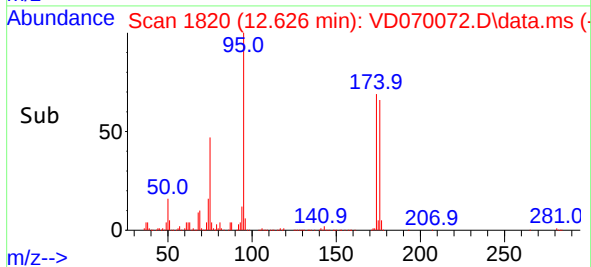
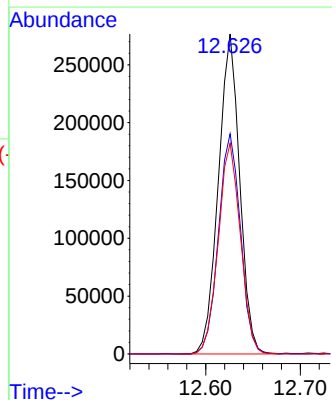
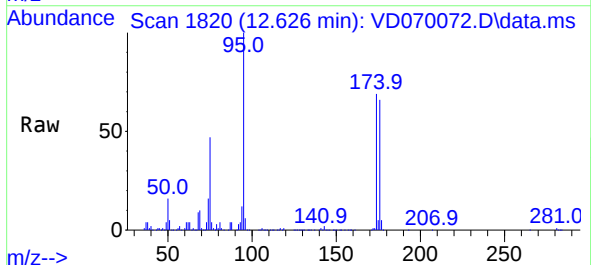


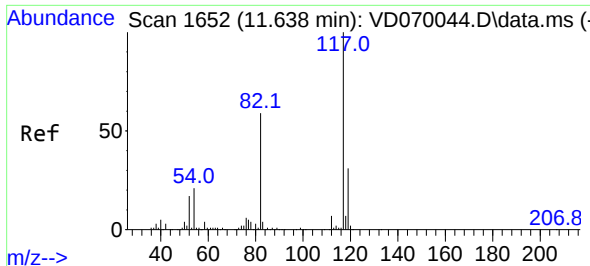

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.638 min Scan# 1652
Delta R.T. -0.000 min
Lab File: VD070072.D
Acq: 16 Aug 2021 17:46

Instrument :
MSVOA_D
ClientSampleId :
SWCS-07-0002

Tgt Ion:117 Resp: 1016205
Ion Ratio Lower Upper
117 100
82 59.3 47.5 71.3
119 31.9 25.1 37.7

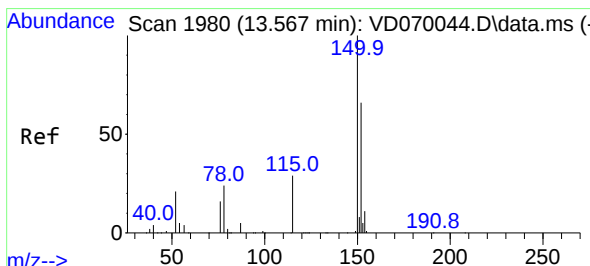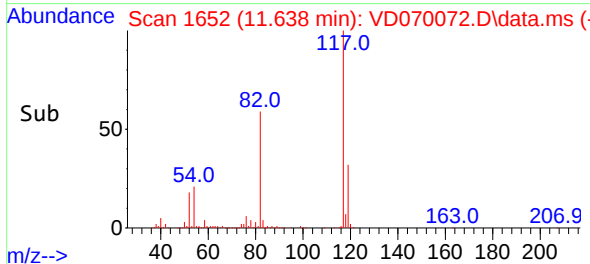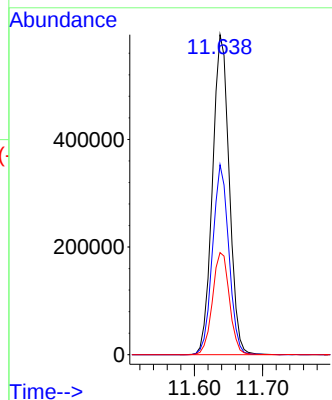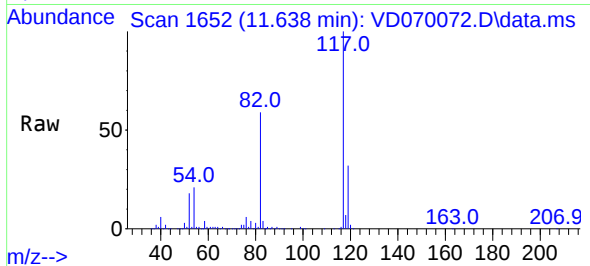

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.567 min Scan# 1980
Delta R.T. -0.000 min
Lab File: VD070072.D
Acq: 16 Aug 2021 17:46

Tgt Ion:152 Resp: 395752
Ion Ratio Lower Upper
152 100
115 62.7 31.2 93.6
150 155.8 0.0 352.0

