


Data Path : Z:\voasrv\HPCHEM1\MSVOA D\Data\VD081920\
 Data File : VD066330.D
 Acq On : 19 Aug 2020 21:22
 Operator : VA/SY
 Sample : BFB
 Misc : 5.00G/5.00ml/MSVOA D/SOIL
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 MSVOA_D
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_D\METHOD\82D080520S.M
 Title : SW846 8260
 Last Update : Wed Aug 05 13:49:25 2020

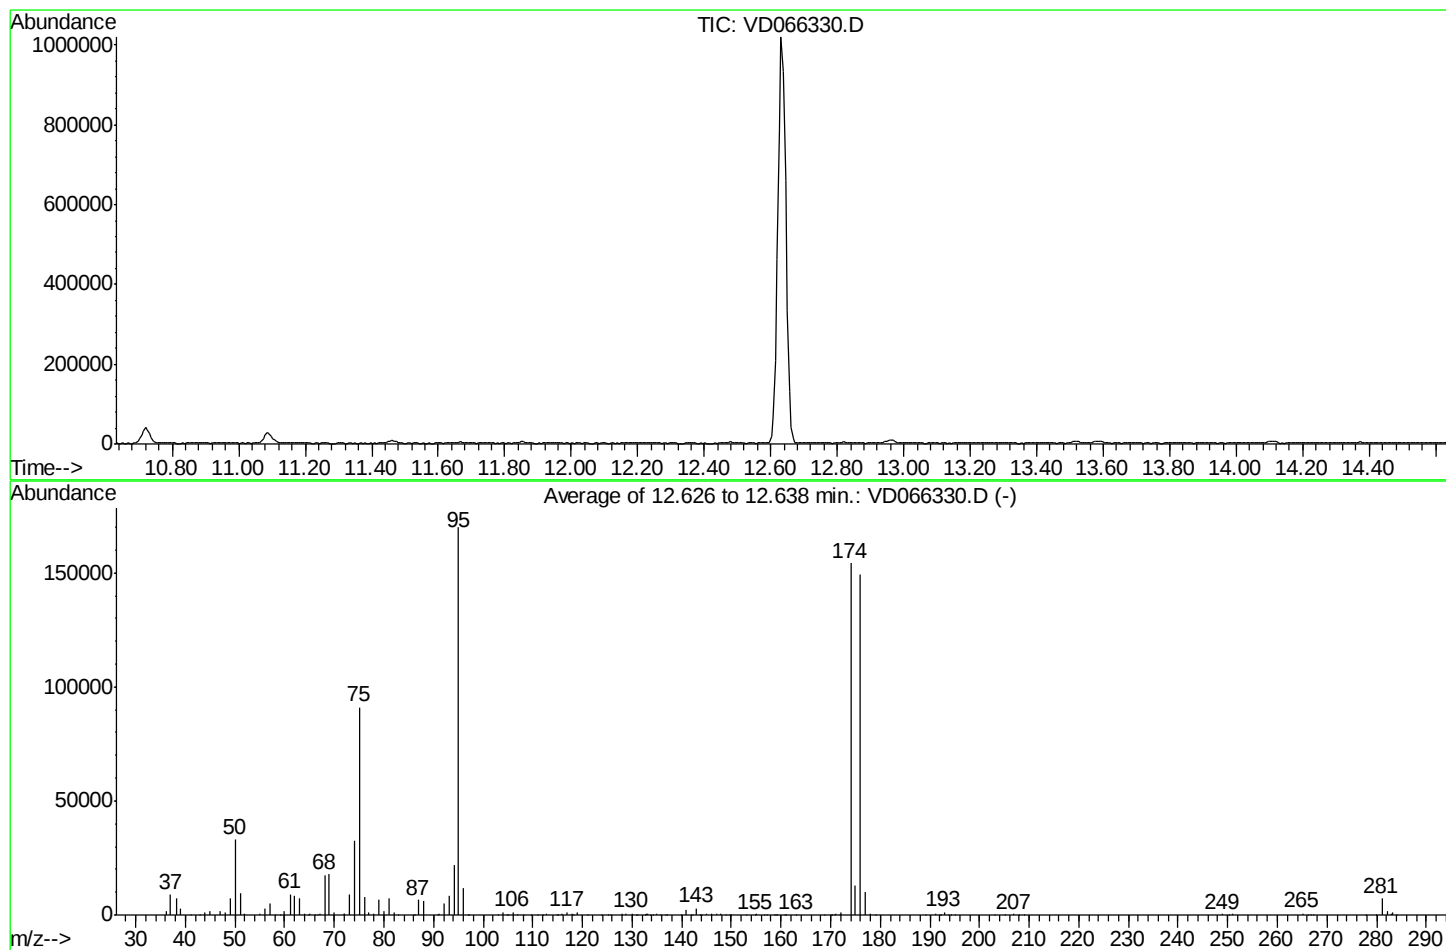

AutoFind: Scans 1820, 1821, 1822; Background Corrected with Scan 1812

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.4	32978	PASS
75	95	30	60	53.6	91181	PASS
95	95	100	100	100.0	169962	PASS
96	95	5	9	6.8	11631	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	100	90.7	154168	PASS
175	174	5	9	8.2	12651	PASS
176	174	95	101	96.8	149301	PASS
177	176	5	9	6.7	9944	PASS