
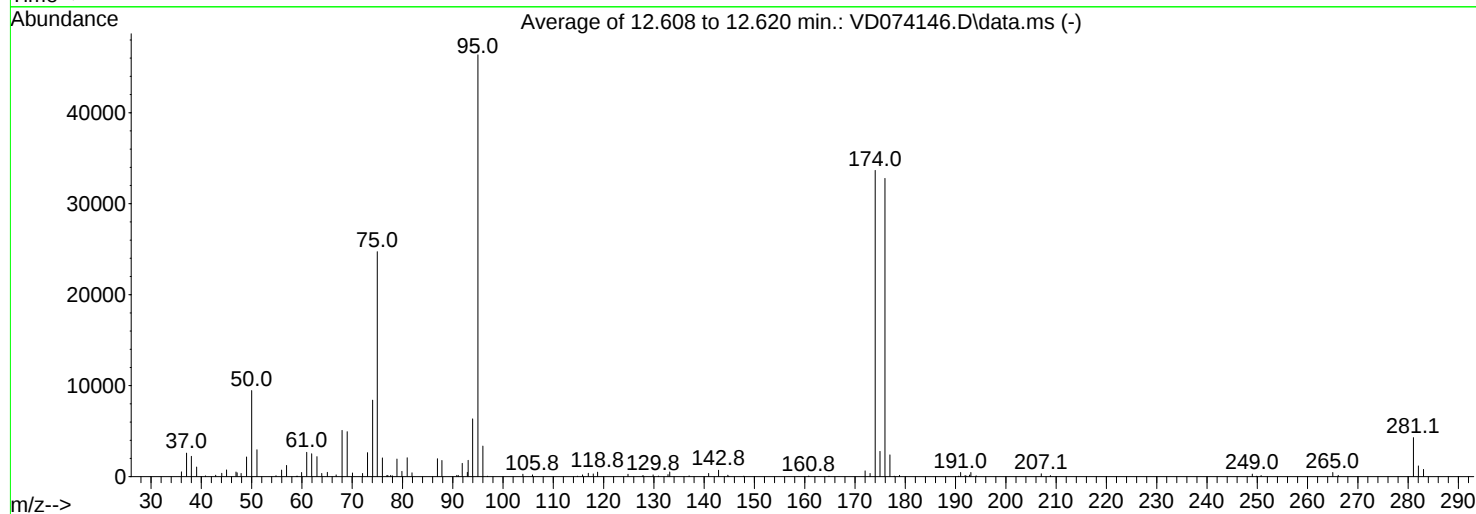


Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD081922\
Data File : VD074146.D
Acq On : 19 Aug 2022 13:31
Operator : VA/SY
Sample : BFB
Misc : 5.00G/5.00ml/MSVOA_D/SOIL
ALS Vial : 2 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D081822S.M
Title : SW846 8260
Last Update : Fri Aug 19 09:25:06 2022

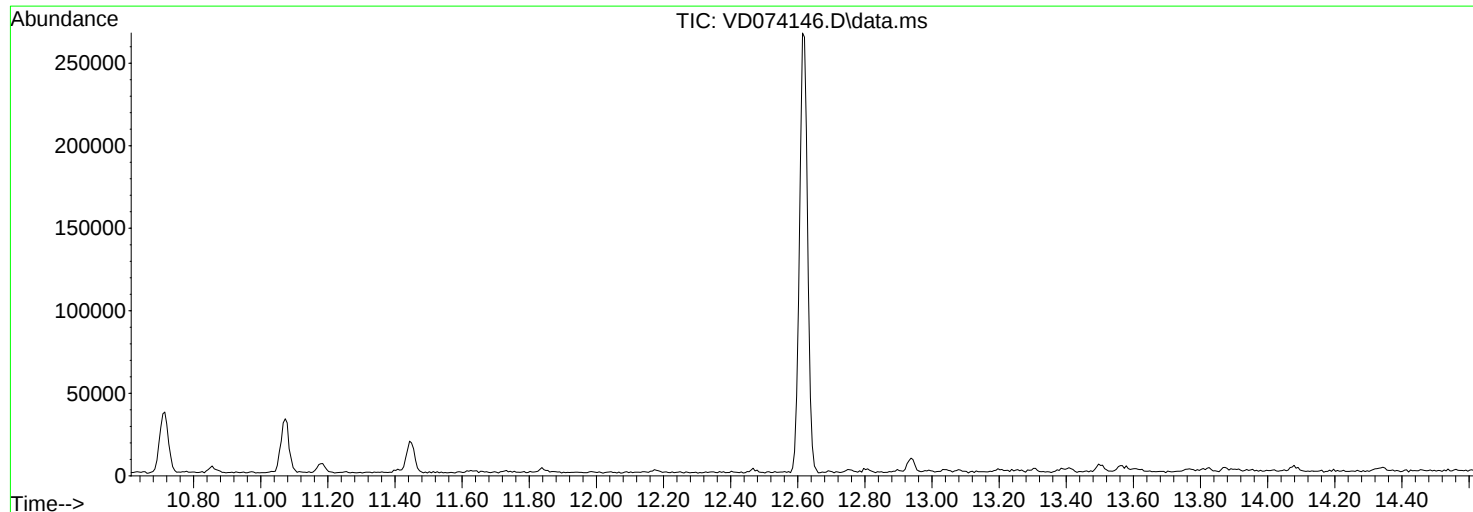

AutoFind: Scans 1817, 1818, 1819; Background Corrected with Scan 1810

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.4	9458	PASS
75	95	30	60	53.3	24733	PASS
95	95	100	100	100.0	46363	PASS
96	95	5	9	7.2	3354	PASS
173	174	0.00	2	1.1	356	PASS
174	95	50	100	72.6	33659	PASS
175	174	5	9	8.3	2786	PASS
176	174	95	101	97.4	32789	PASS
177	176	5	9	7.3	2393	PASS