


Data Path : Z:\voasrv\HPCHEM1\MSVOA D\Data\VD082720\
 Data File : VD066428.D
 Acq On : 27 Aug 2020 10:37
 Operator : VA/SY
 Sample : BFB
 Misc : 5.00G/5.00ml/MSVOA D/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_D
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_D\METHOD\82D082120S.M
 Title : SW846 8260
 Last Update : Fri Aug 21 13:36:12 2020

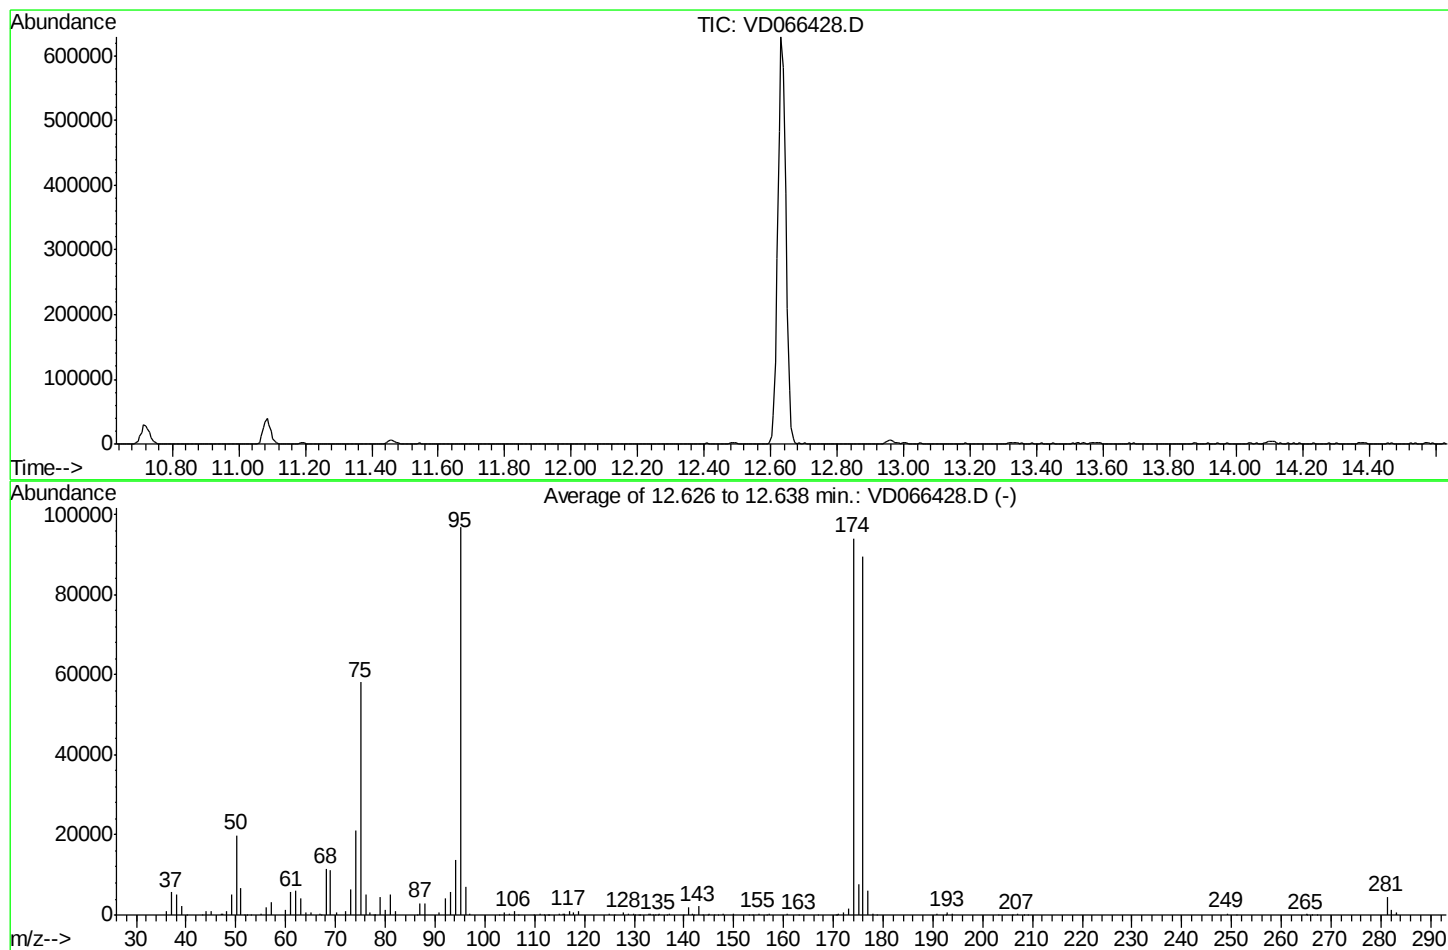

AutoFind: Scans 1820, 1821, 1822; Background Corrected with Scan 1812

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.5	19810	PASS
75	95	30	60	60.0	58050	PASS
95	95	100	100	100.0	96757	PASS
96	95	5	9	7.4	7150	PASS
173	174	0.00	2	1.9	1756	PASS
174	95	50	100	97.2	94061	PASS
175	174	5	9	8.2	7753	PASS
176	174	95	101	95.2	89565	PASS
177	176	5	9	6.9	6173	PASS