


Data Path : Z:\VOASRV\HPCHEM1\MSVOA D\DATA\VD091420\
 Data File : VD066678.D
 Acq On : 14 Sep 2020 17:54
 Operator : VA/SY
 Sample : BFB
 Misc : 5.00G/5.00ml/MSVOA D/SOIL
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_D
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_D\METHOD\82D090320S.M
 Title : SW846 8260
 Last Update : Fri Sep 04 01:57:04 2020

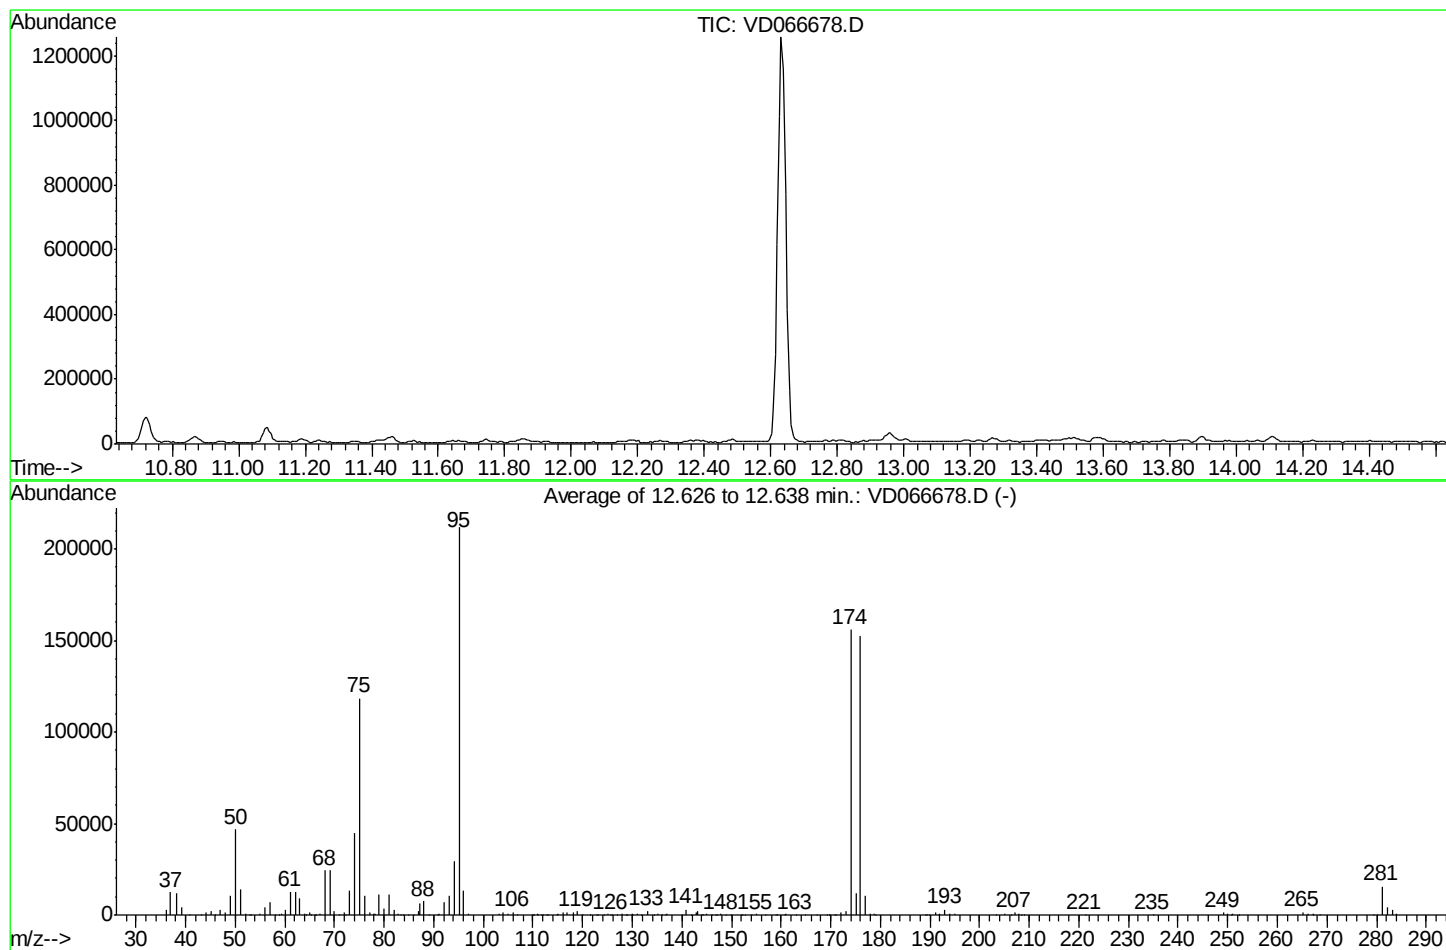

AutoFind: Scans 1820, 1821, 1822; Background Corrected with Scan 1812

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	22.0	46568	PASS
75	95	30	60	55.8	118322	PASS
95	95	100	100	100.0	211868	PASS
96	95	5	9	6.3	13395	PASS
173	174	0.00	2	1.5	2260	PASS
174	95	50	100	73.5	155733	PASS
175	174	5	9	7.8	12166	PASS
176	174	95	101	98.1	152778	PASS
177	176	5	9	6.8	10366	PASS