
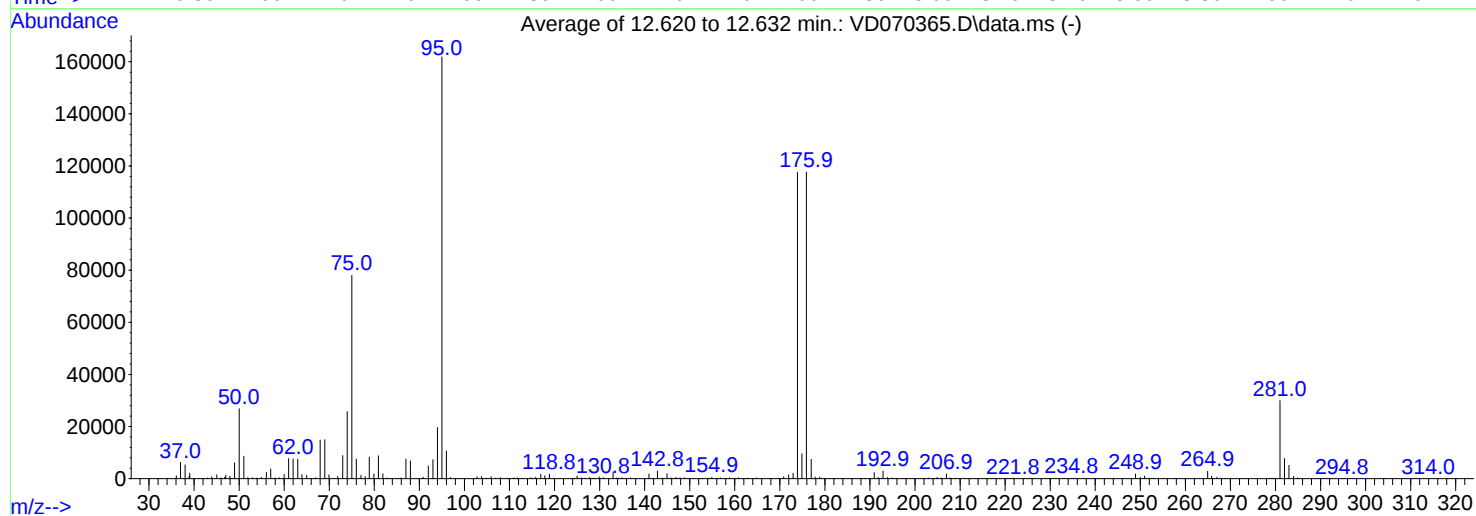


Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD091521\
Data File : VD070365.D
Acq On : 15 Sep 2021 08:47
Operator : VA/SY
Sample : BFB
Misc : 5.00G/5.00ml/MSVOA_D/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D090821S.M
Title : SW846 8260
Last Update : Thu Sep 09 03:07:09 2021

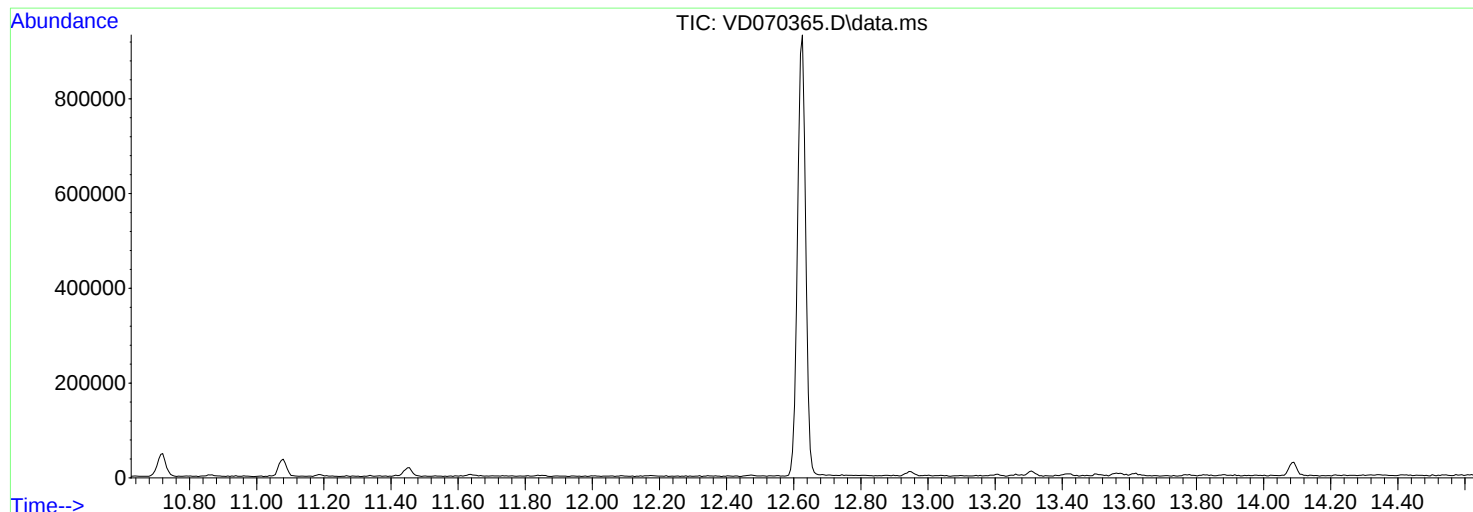

AutoFind: Scans 1819, 1820, 1821; Background Corrected with Scan 1809

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.6	26816	PASS
75	95	30	60	48.2	78008	PASS
95	95	100	100	100.0	161877	PASS
96	95	5	9	6.5	10601	PASS
173	174	0.00	2	1.8	2064	PASS
174	95	50	100	72.6	117589	PASS
175	174	5	9	8.1	9533	PASS
176	174	95	101	100.0	117624	PASS
177	176	5	9	6.3	7430	PASS