
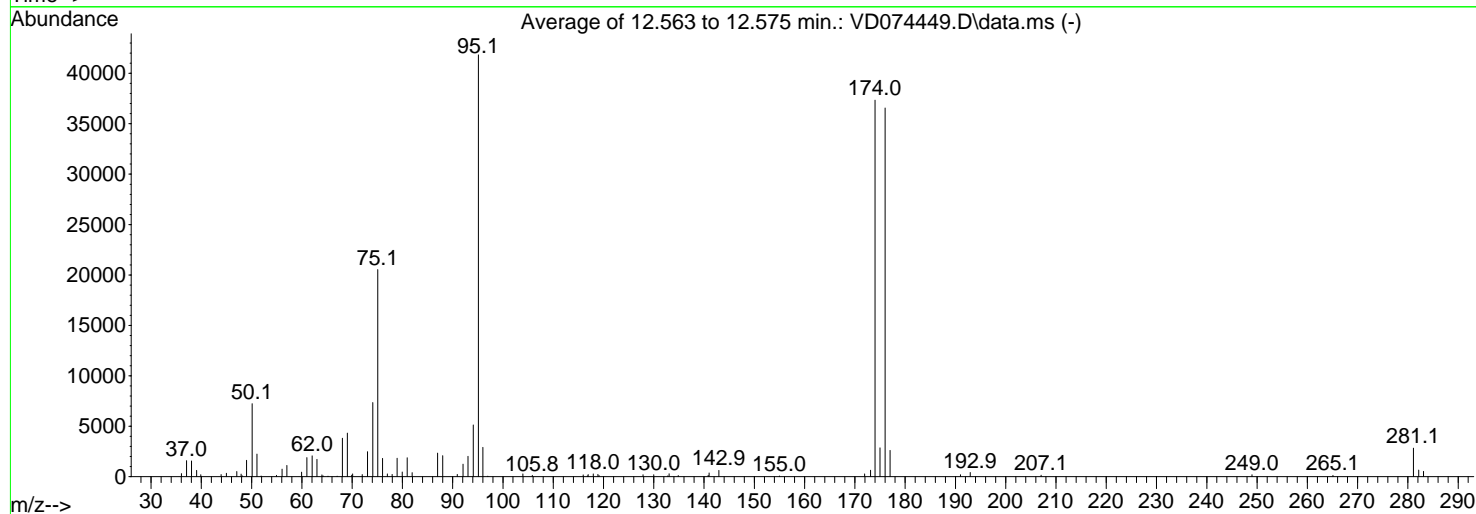


Data Path : Z:\voasrv\HPCHEM1\MSVOA\_D\Data\VD100522\  
 Data File : VD074449.D  
 Acq On : 05 Oct 2022 12:03  
 Operator : VA/SY  
 Sample : BFB  
 Misc : 5.00G/5.00ml/MSVOA\_D/SOIL  
 ALS Vial : 1 Sample Multiplier: 1

Instrument :  
 MSVOA\_D  
 ClientSampleId :  
 BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA\_D\Method\82D100522S.M  
 Title : SW846 8260  
 Last Update : Thu Oct 06 01:54:40 2022

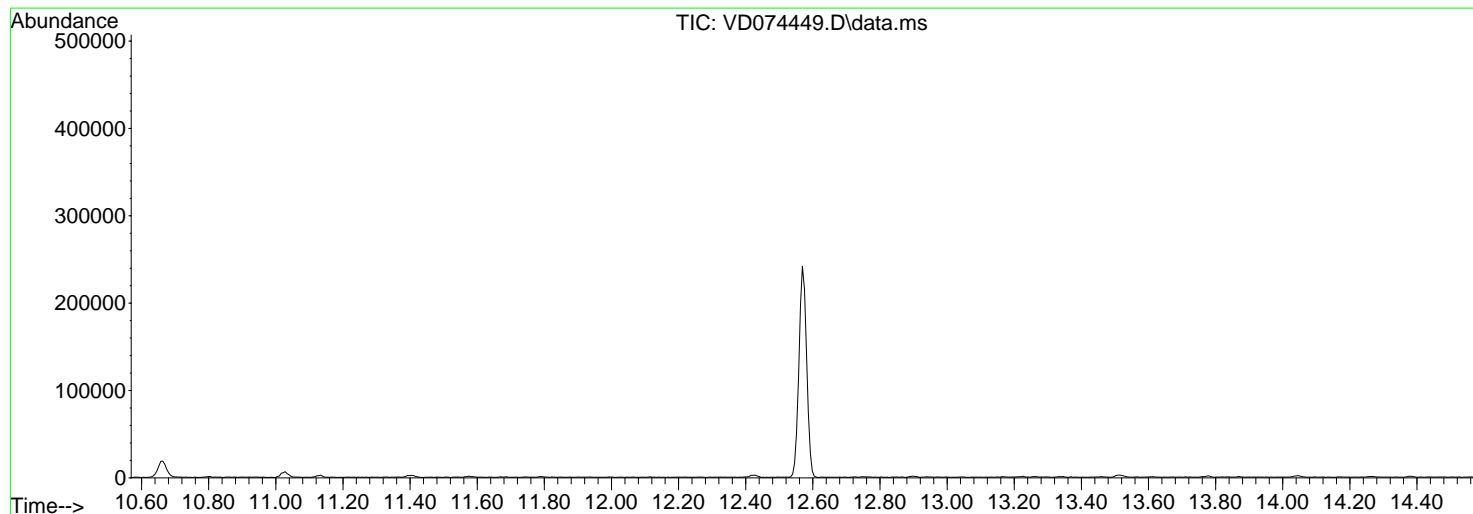

AutoFind: Scans 1866, 1867, 1868; Background Corrected with Scan 1858

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.3	7243	PASS
75	95	30	60	49.1	20533	PASS
95	95	100	100	100.0	41832	PASS
96	95	5	9	6.9	2907	PASS
173	174	0.00	2	1.7	633	PASS
174	95	50	100	89.3	37344	PASS
175	174	5	9	7.6	2854	PASS
176	174	95	101	97.9	36555	PASS
177	176	5	9	7.1	2602	PASS