


Data Path : Z:\voasrv\HPCHEM1\MSVOA D\Data\VD100720\
Data File : VD067164.D
Acq On : 07 Oct 2020 21:03
Operator : VA/SY
Sample : BFB
Misc : 5.00G/5.00ml/MSVOA D/SOIL
ALS Vial : 26 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_D\METHOD\82D100120S.M
Title : SW846 8260
Last Update : Thu Oct 01 15:19:17 2020

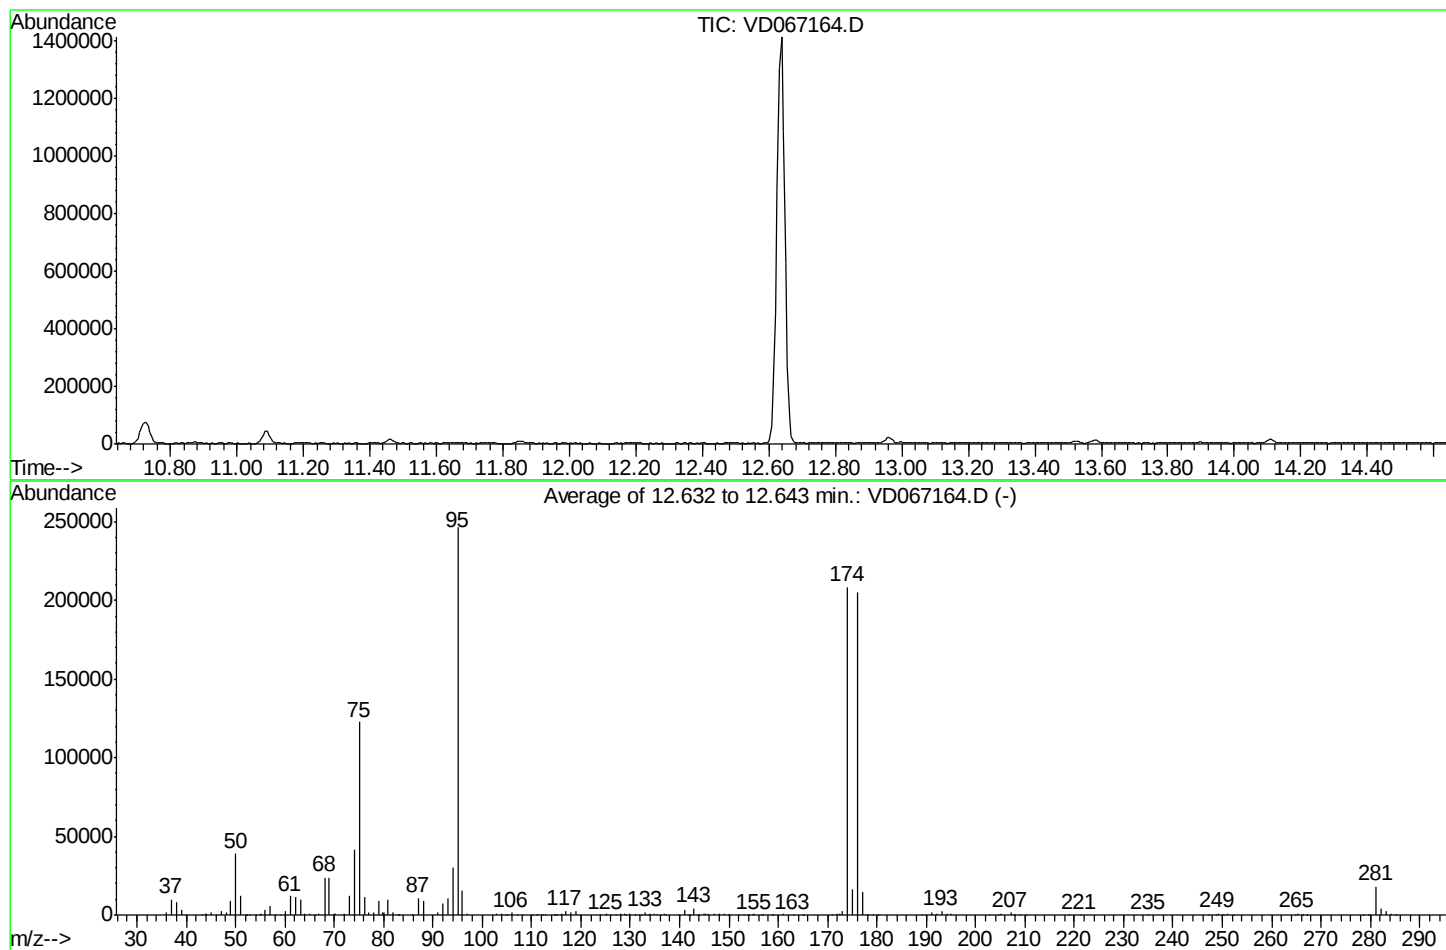

AutoFind: Scans 1821, 1822, 1823; Background Corrected with Scan 1812

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	15.8	38928	PASS
75	95	30	60	49.7	122589	PASS
95	95	100	100	100.0	246464	PASS
96	95	5	9	6.2	15219	PASS
173	174	0.00	2	1.2	2501	PASS
174	95	50	100	84.6	208554	PASS
175	174	5	9	7.7	16009	PASS
176	174	95	101	98.2	204842	PASS
177	176	5	9	7.0	14338	PASS