


Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD101221\
Data File : VD070670.D
Acq On : 12 Oct 2021 10:33
Operator : VA/SY
Sample : BFB
Misc : 5.00G/5.00ml/MSVOA_D/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D100521S.M
Title : SW846 8260
Last Update : Wed Oct 06 09:10:31 2021

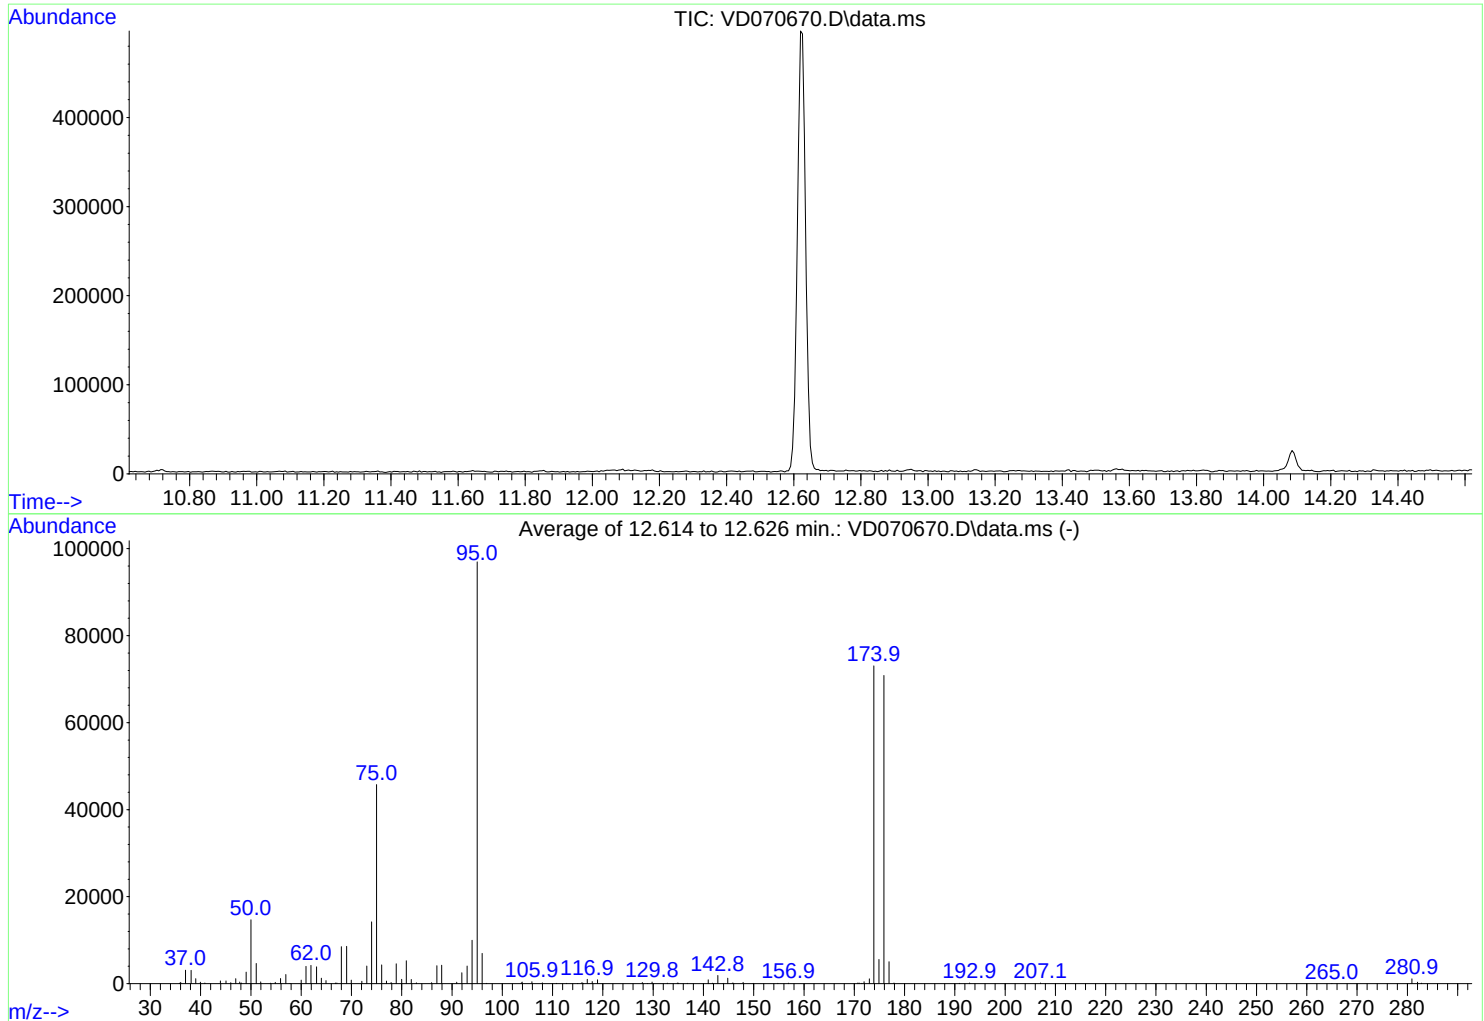

AutoFind: Scans 1818, 1819, 1820; Background Corrected with Scan 1811

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	15.2	14695	PASS
75	95	30	60	47.2	45776	PASS
95	95	100	100	100.0	96968	PASS
96	95	5	9	7.2	6939	PASS
173	174	0.00	2	1.5	1100	PASS
174	95	50	100	75.3	73061	PASS
175	174	5	9	7.6	5549	PASS
176	174	95	101	97.0	70856	PASS
177	176	5	9	7.1	5030	PASS