
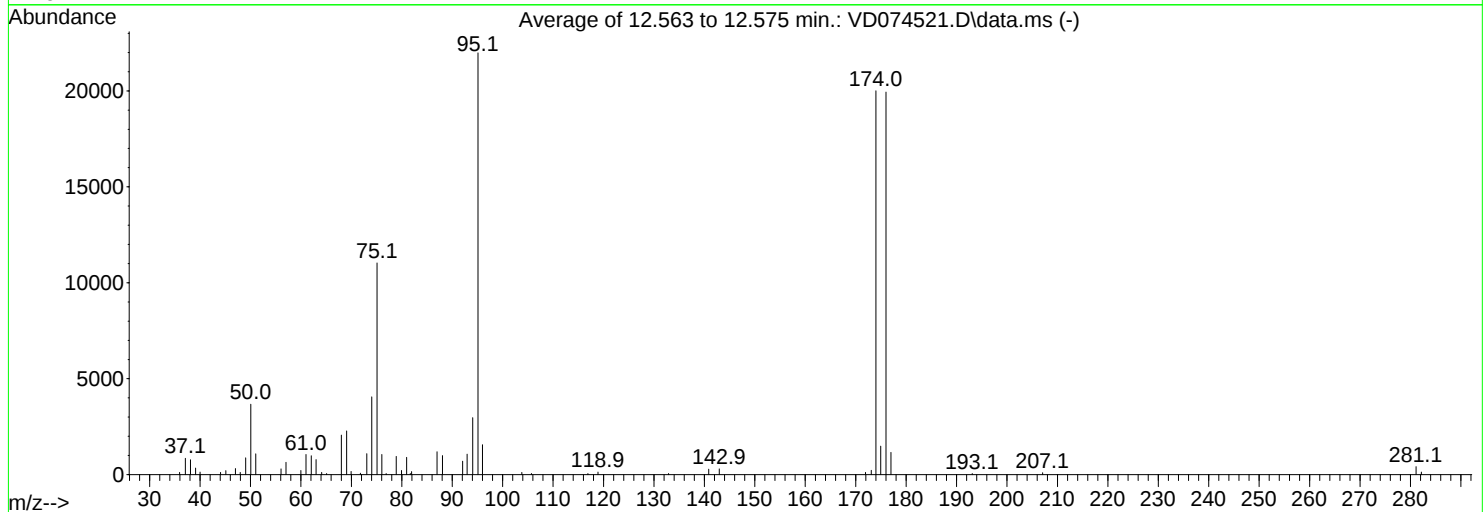


Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD101322\
Data File : VD074521.D
Acq On : 13 Oct 2022 09:52
Operator : VA/SY
Sample : BFB
Misc : 5.00G/5.00ml/MSVOA_D/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D101122S.M
Title : SW846 8260
Last Update : Wed Oct 12 13:14:00 2022

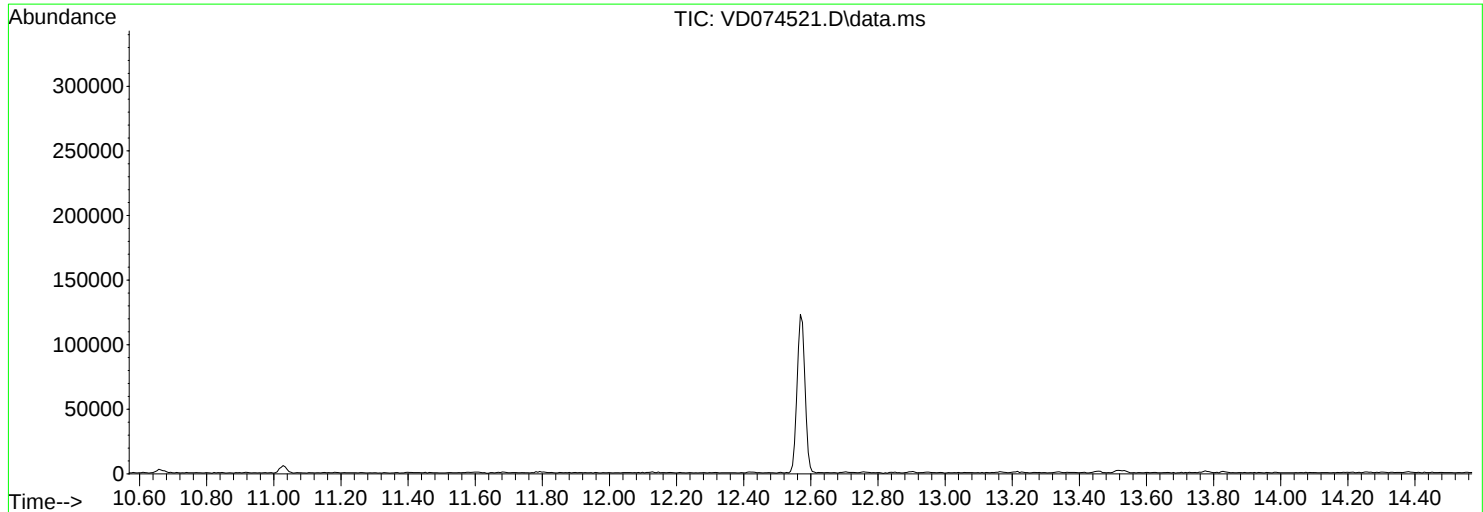

AutoFind: Scans 1866, 1867, 1868; Background Corrected with Scan 1859

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	16.7	3667	PASS
75	95	30	60	50.2	11034	PASS
95	95	100	100	100.0	21984	PASS
96	95	5	9	7.1	1557	PASS
173	174	0.00	2	1.1	227	PASS
174	95	50	100	91.0	20003	PASS
175	174	5	9	7.4	1482	PASS
176	174	95	101	99.7	19939	PASS
177	176	5	9	5.8	1159	PASS