


Data Path : Z:\voasrv\HPCHEM1\MSVOA D\Data\VD101719\
Data File : VD063994.D
Acq On : 17 Oct 2019 09:37
Operator : VA/SY
Sample : BFB
Misc : 5.00G/5.00ml/MSVOA D/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_D\METHOD\82D100219S.M
Title : SW846 8260
Last Update : Sat Oct 05 03:51:17 2019

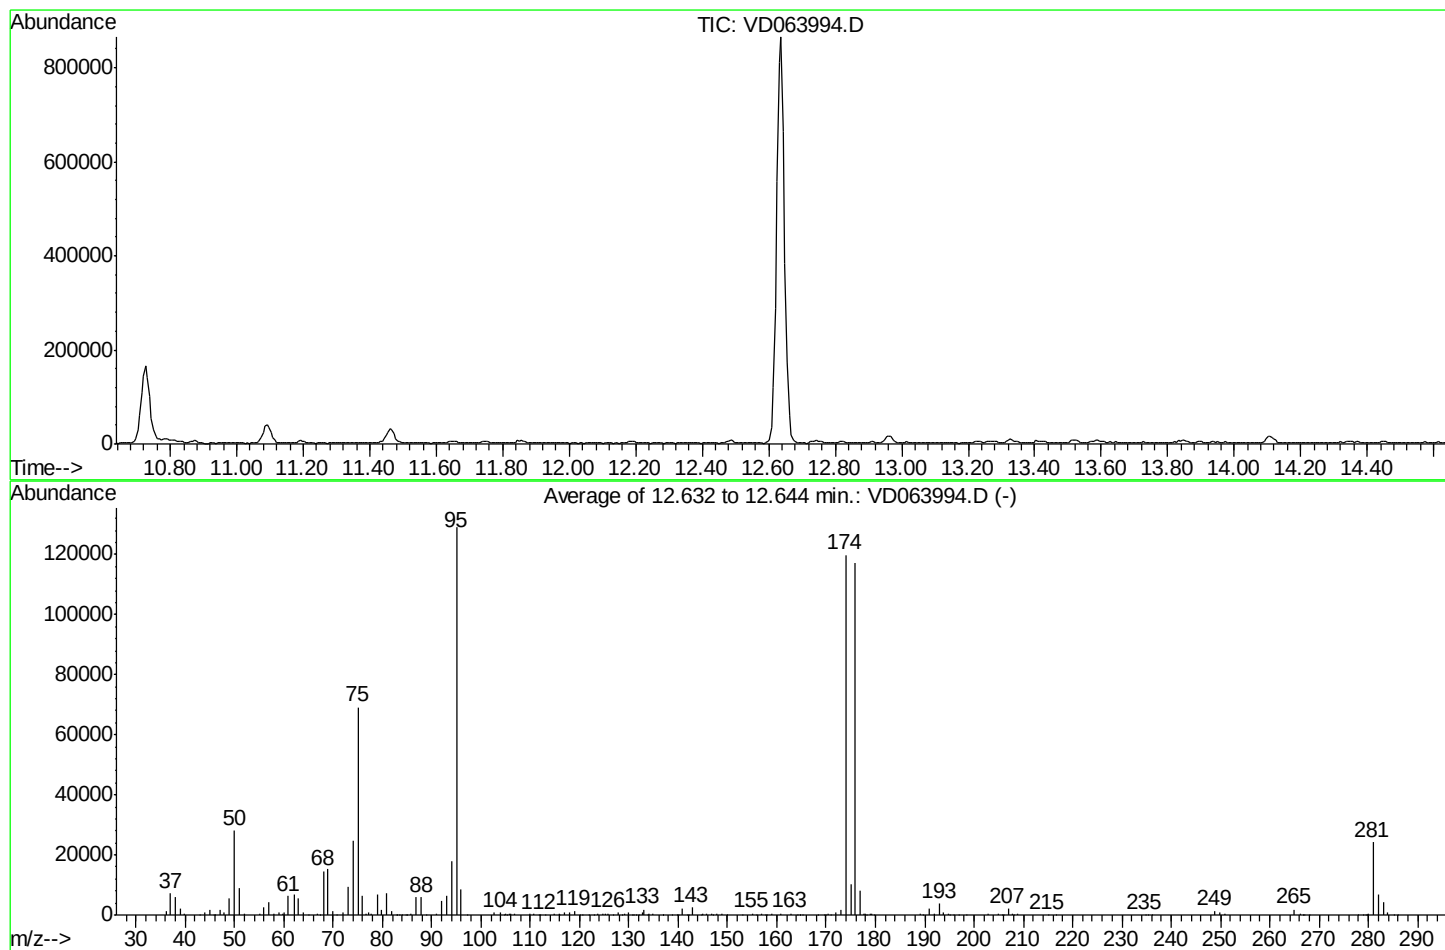

AutoFind: Scans 1821, 1822, 1823; Background Corrected with Scan 1812

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	21.8	28077	PASS
75	95	30	60	53.5	69120	PASS
95	95	100	100	100.0	129080	PASS
96	95	5	9	6.5	8369	PASS
173	174	0.00	2	1.5	1765	PASS
174	95	50	100	92.8	119778	PASS
175	174	5	9	8.5	10189	PASS
176	174	95	101	97.9	117224	PASS
177	176	5	9	7.0	8218	PASS