


Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD101822\
 Data File : VD074556.D
 Acq On : 18 Oct 2022 09:15
 Operator : VA/SY
 Sample : BFB
 Misc : 5.00G/5.00ml/MSVOA_D/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_D
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D101122S.M
 Title : SW846 8260
 Last Update : Wed Oct 12 13:14:00 2022

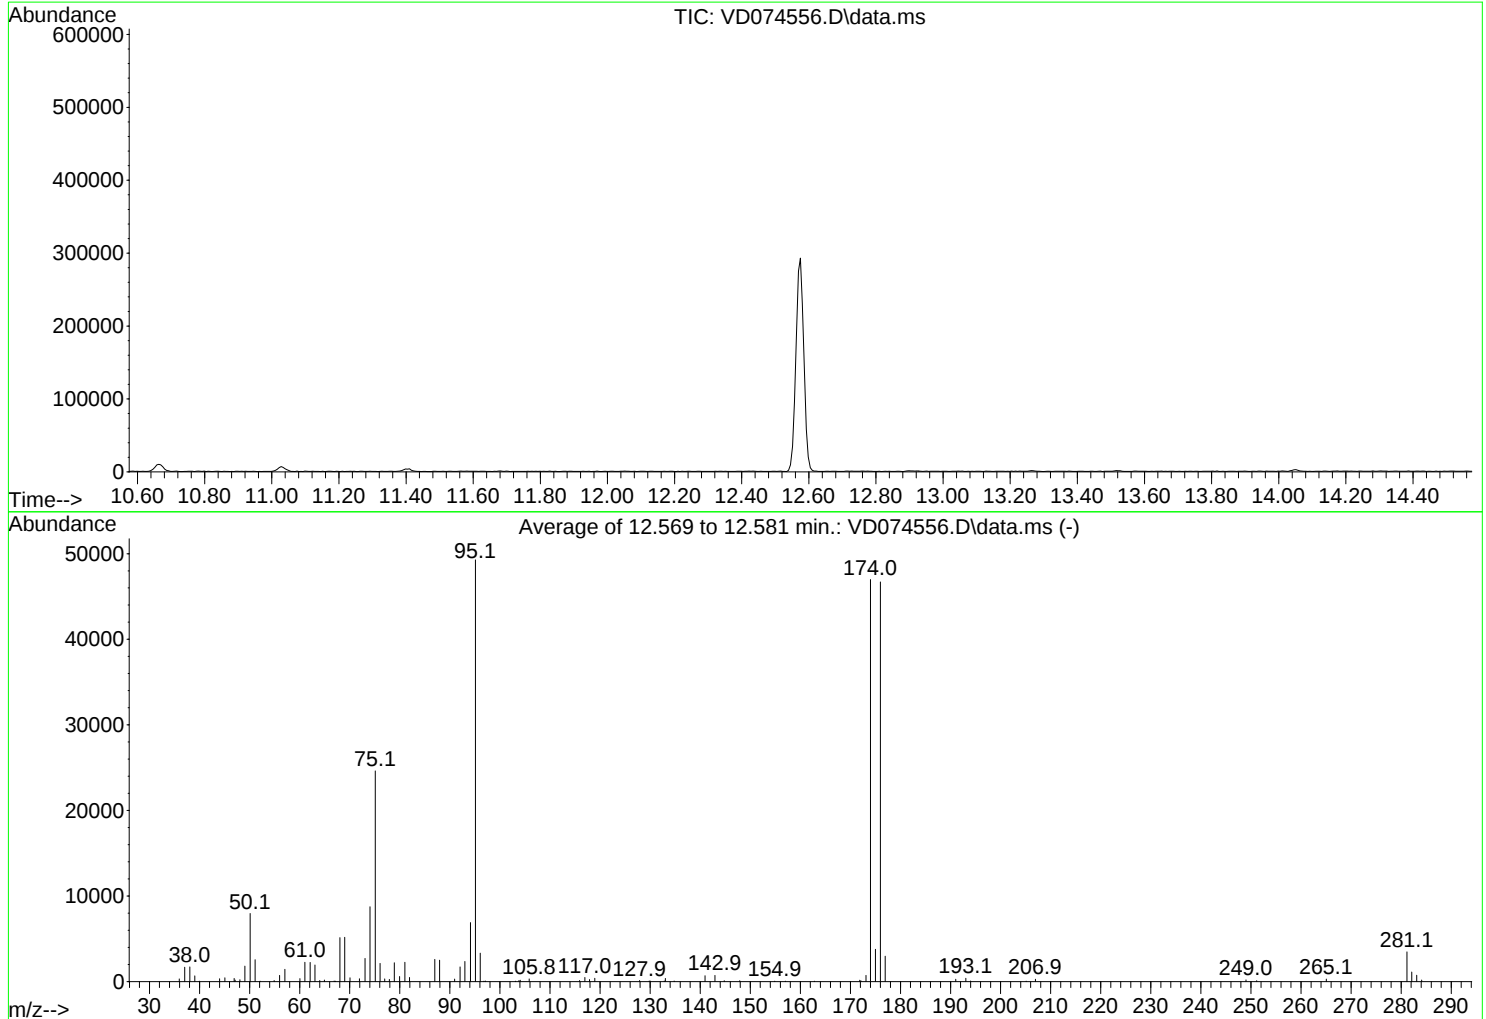

AutoFind: Scans 1867, 1868, 1869; Background Corrected with Scan 1859

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.2	7972	PASS
75	95	30	60	50.0	24619	PASS
95	95	100	100	100.0	49285	PASS
96	95	5	9	6.7	3323	PASS
173	174	0.00	2	1.5	725	PASS
174	95	50	100	95.3	46987	PASS
175	174	5	9	8.0	3773	PASS
176	174	95	101	99.4	46701	PASS
177	176	5	9	6.4	2970	PASS