

Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD102021\
 Data File : VD070781.D
 Acq On : 20 Oct 2021 17:46
 Operator : VA/SY
 Sample : M4287-01
 Misc : 6.36G/5.00ml/MSVOA_D/SOIL
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_D
 ClientSampleId :
 EXC-SOIL-A

Quant Time: Oct 21 05:40:25 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D101521S.M
 Quant Title : SW846 8260
 QLast Update : Mon Oct 18 08:32:03 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	7.979	168	525300	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	8.861	114	977252	50.00	ug/l	0.00
63) Chlorobenzene-d5	11.638	117	926401	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.561	152	396364	50.00	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.326	65	356775	57.34	ug/l	0.00
Spiked Amount	50.000	Range	50 - 163	Recovery	=	114.68%
35) Dibromofluoromethane	7.908	113	318358	50.88	ug/l	0.00
Spiked Amount	50.000	Range	54 - 147	Recovery	=	101.76%
50) Toluene-d8	10.332	98	1251342	52.17	ug/l	0.00
Spiked Amount	50.000	Range	49 - 140	Recovery	=	104.34%
62) 4-Bromofluorobenzene	12.626	95	443851	53.74	ug/l	0.00
Spiked Amount	50.000	Range	25 - 144	Recovery	=	107.48%


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD102021\
Data File : VD070781.D
Acq On : 20 Oct 2021 17:46
Operator : VA/SY
Sample : M4287-01
Misc : 6.36G/5.00ml/MSVOA_D/SOIL
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
EXC-SOIL-A

Quant Time: Oct 21 05:40:25 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D101521S.M
Quant Title : SW846 8260
QLast Update : Mon Oct 18 08:32:03 2021
Response via : Initial Calibration




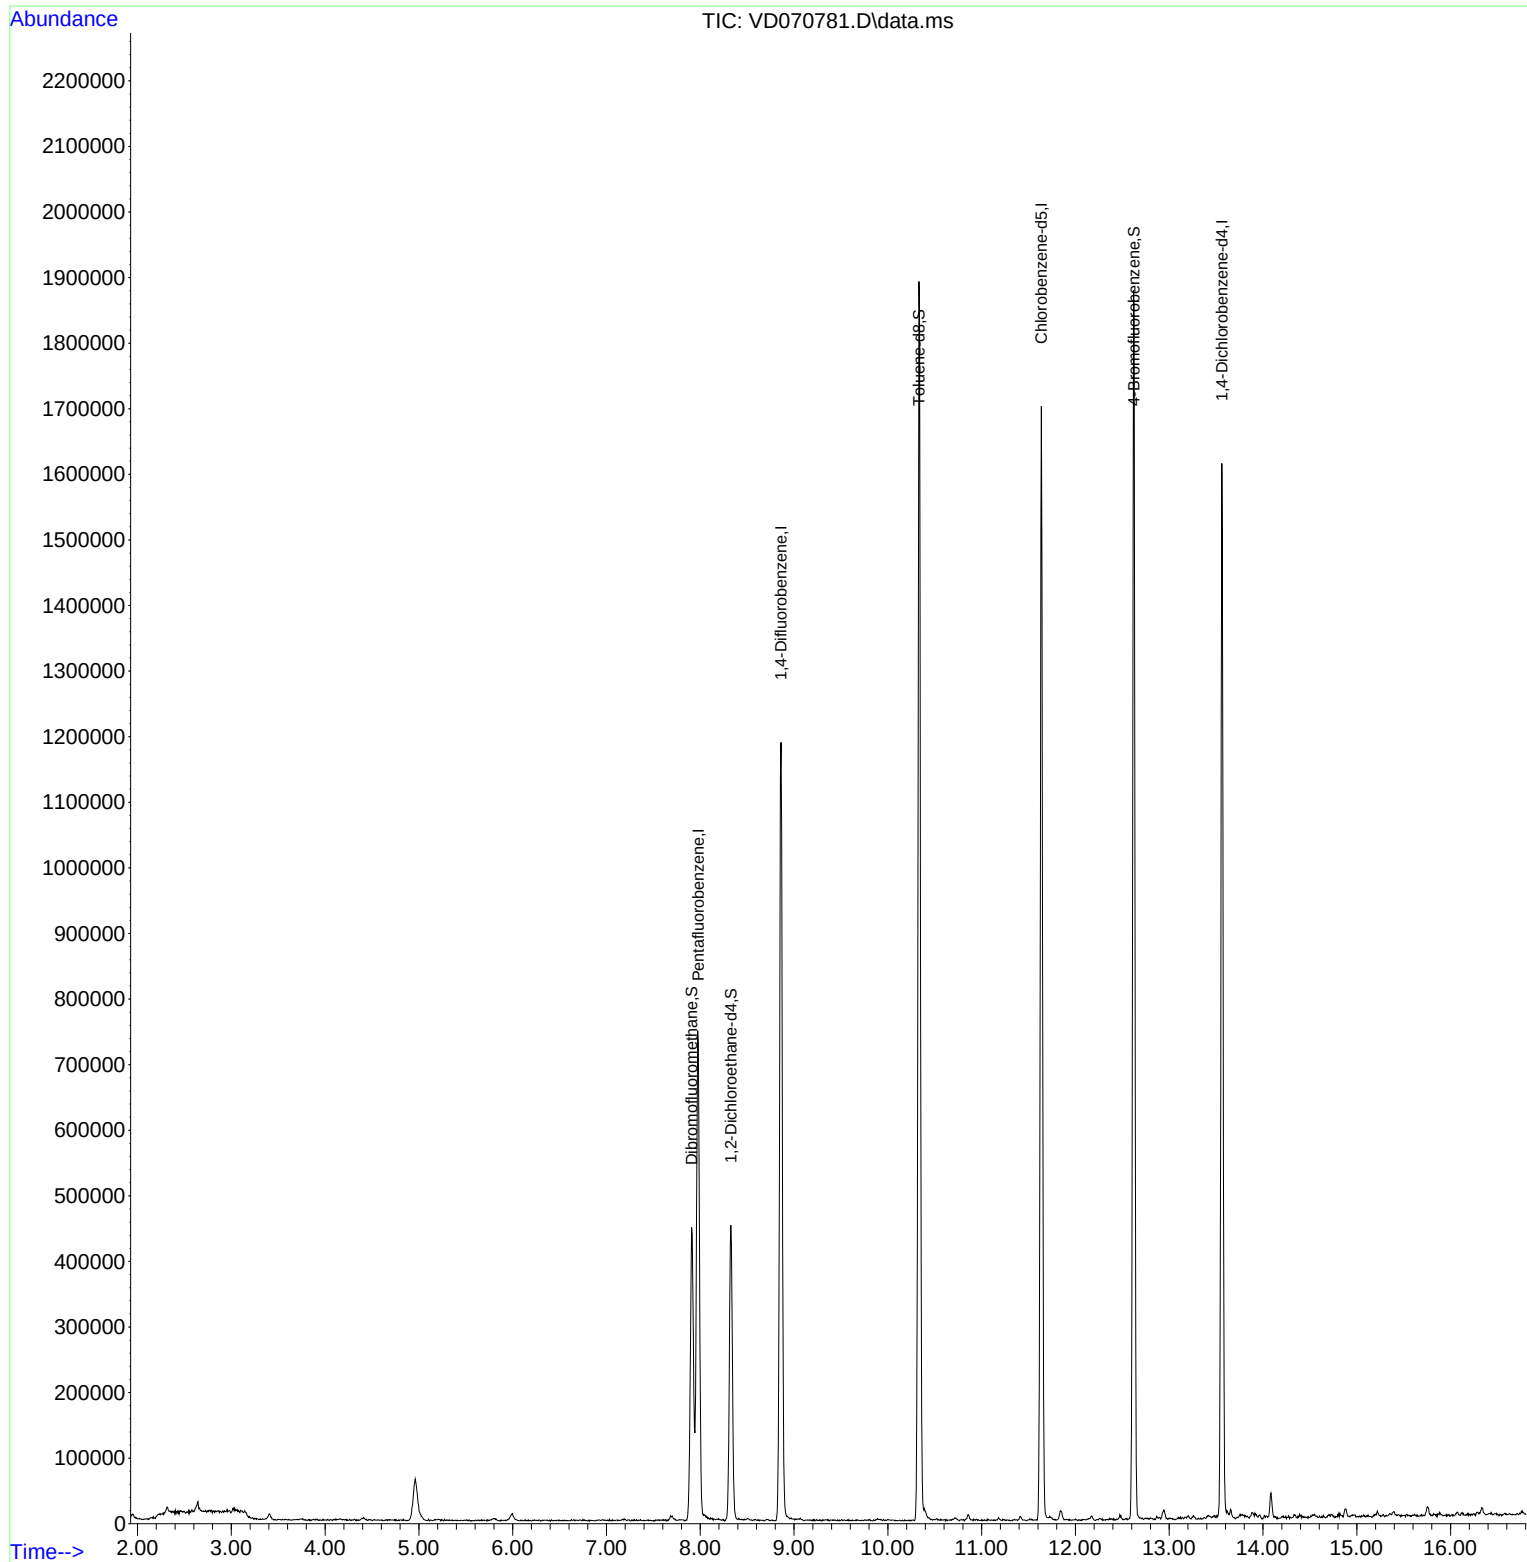


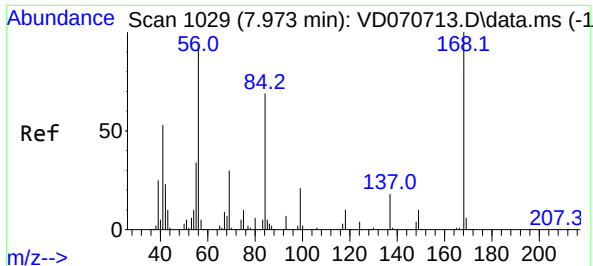

#1
Pentafluorobenzene
Concen: 50.00 ug/l
RT: 7.979 min Scan# 1030
Delta R.T. 0.006 min
Lab File: VD070781.D
Acq: 20 Oct 2021 17:46




Instrument :
MSVOA_D
ClientSampleId :
EXC-SOIL-A


Tgt Ion:168 Resp: 525300
Ion Ratio Lower Upper
168 100
99 58.5 51.4 77.0

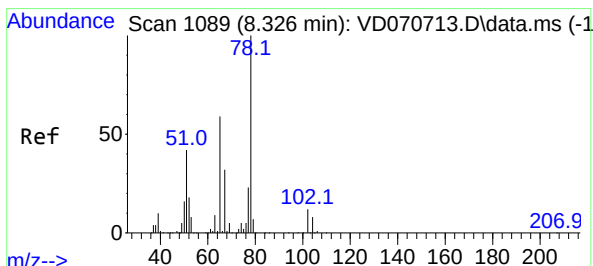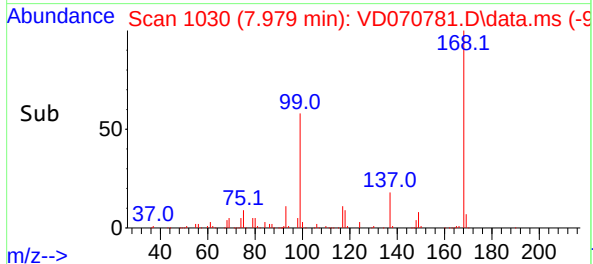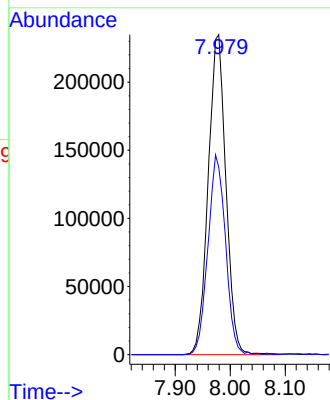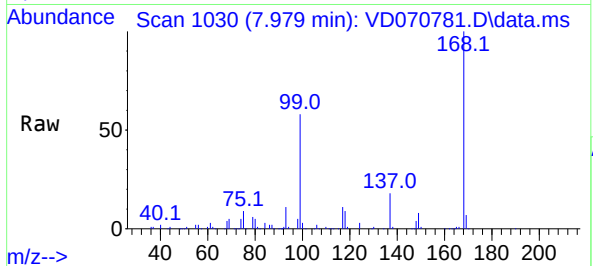

#33
1,2-Dichloroethane-d4
Concen: 57.34 ug/l
RT: 8.326 min Scan# 1089
Delta R.T. 0.000 min
Lab File: VD070781.D
Acq: 20 Oct 2021 17:46

Tgt Ion: 65 Resp: 356775
Ion Ratio Lower Upper
65 100
67 54.2 0.0 110.2

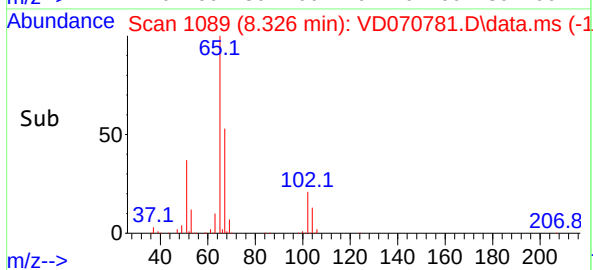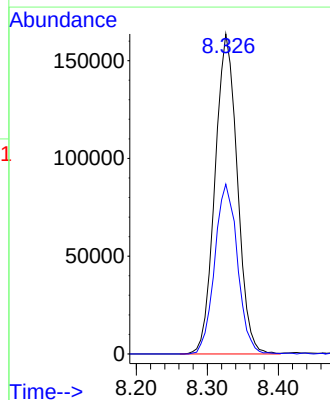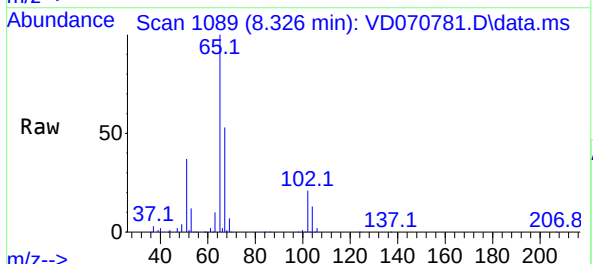




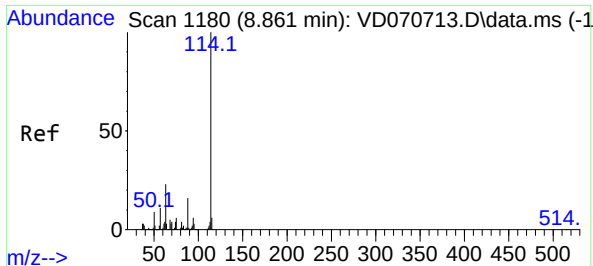


#34

1,4-Difluorobenzene
Concen: 50.00 ug/l
RT: 8.861 min Scan# 1180
Delta R.T. 0.000 min
Lab File: VD070781.D
Acq: 20 Oct 2021 17:46

Instrument :
MSVOA_D
ClientSampleId :
EXC-SOIL-A




Tgt Ion:114 Resp: 977252
Ion Ratio Lower Upper
114 100
63 22.9 0.0 41.8
88 16.8 0.0 32.6

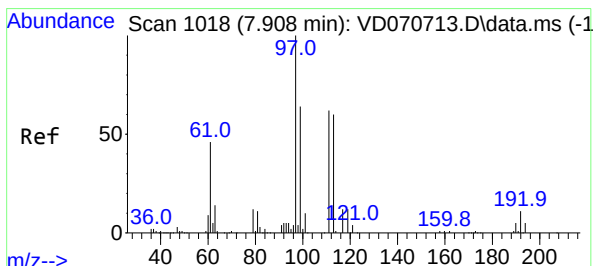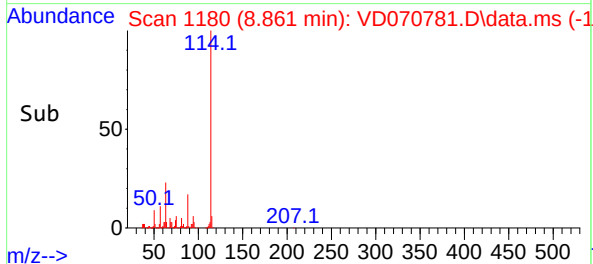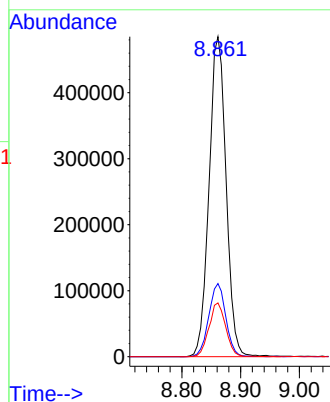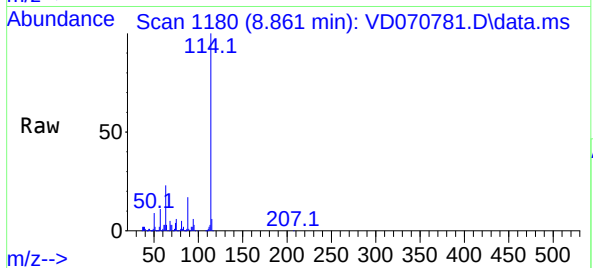


#35

Dibromofluoromethane
Concen: 50.88 ug/l
RT: 7.908 min Scan# 1018
Delta R.T. 0.000 min
Lab File: VD070781.D
Acq: 20 Oct 2021 17:46

Tgt Ion:113 Resp: 318358
Ion Ratio Lower Upper
113 100
111 102.8 83.1 124.7
192 18.9 12.7 19.1


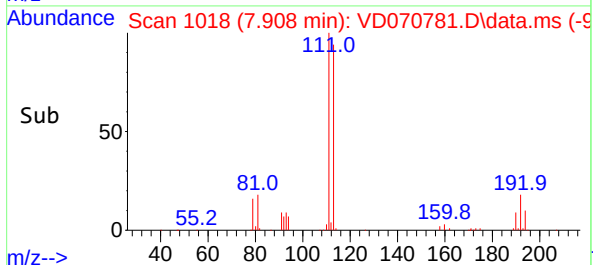
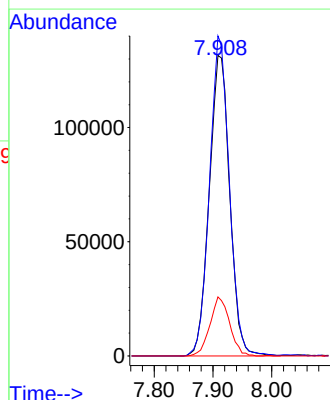
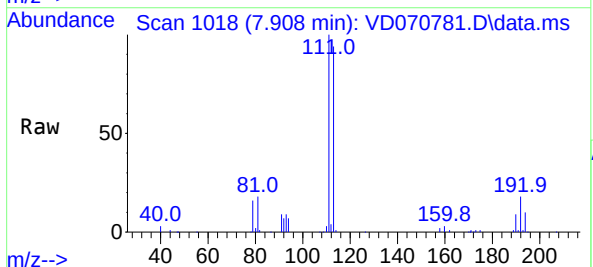


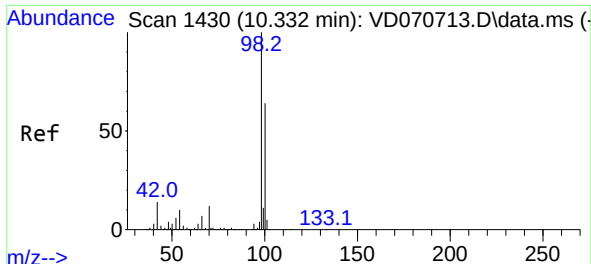

#50
Toluene-d8
Concen: 52.17 ug/l
RT: 10.332 min Scan# 1430
Delta R.T. 0.000 min
Lab File: VD070781.D
Acq: 20 Oct 2021 17:46




Instrument :
MSVOA_D
ClientSampleId :
EXC-SOIL-A


Tgt Ion: 98 Resp: 1251342
Ion Ratio Lower Upper
98 100
100 64.2 52.2 78.4

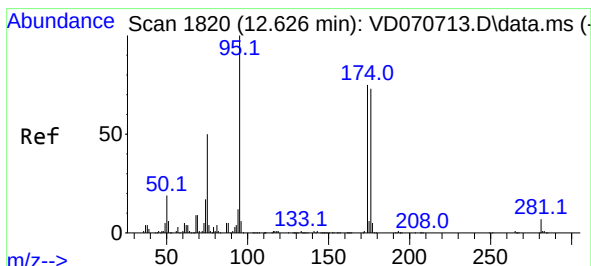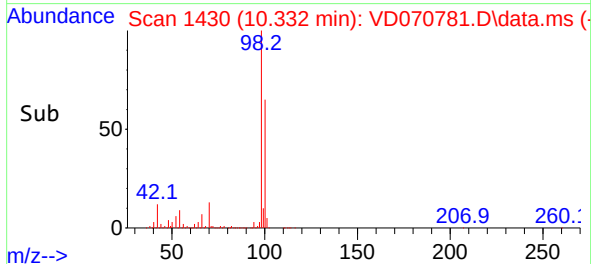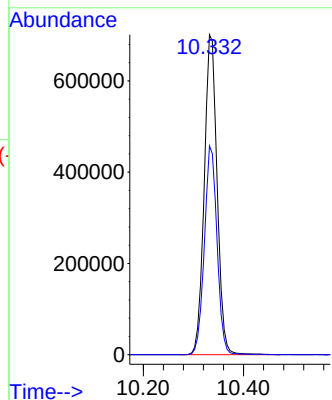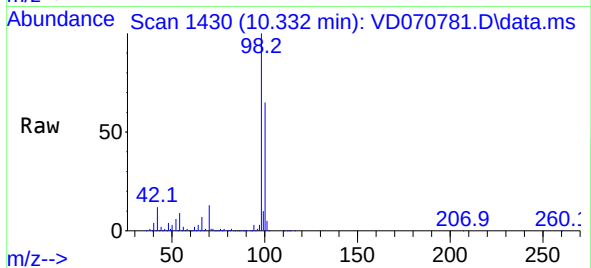

#62
4-Bromofluorobenzene
Concen: 53.74 ug/l
RT: 12.626 min Scan# 1820
Delta R.T. 0.000 min
Lab File: VD070781.D
Acq: 20 Oct 2021 17:46

Tgt Ion: 95 Resp: 443851
Ion Ratio Lower Upper
95 100
174 73.7 0.0 138.0
176 70.4 0.0 135.6


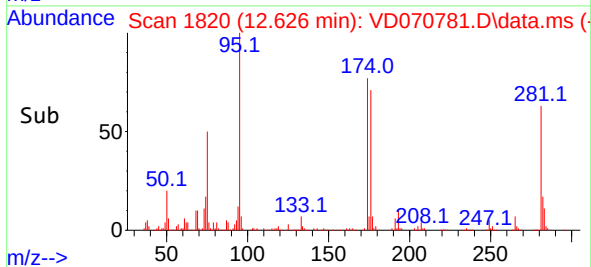
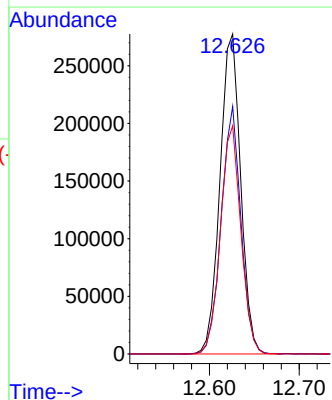
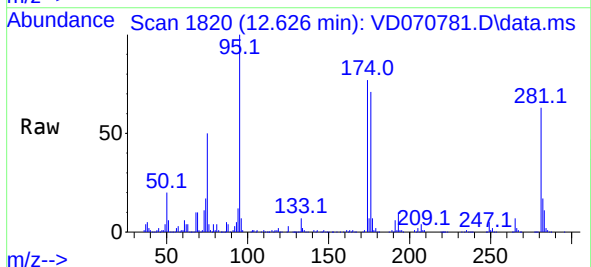


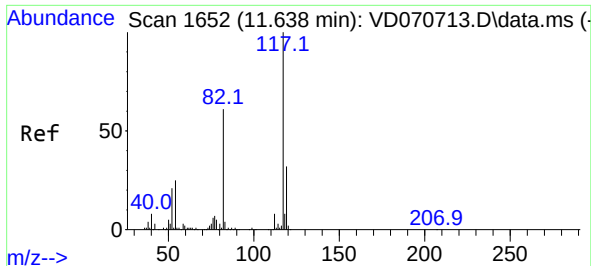

#63
Chlorobenzene-d5
Concen: 50.00 ug/l
RT: 11.638 min Scan# 1652
Delta R.T. 0.000 min
Lab File: VD070781.D
Acq: 20 Oct 2021 17:46

Instrument :
MSVOA_D
ClientSampleId :
EXC-SOIL-A

Tgt Ion:117 Resp: 926401
Ion Ratio Lower Upper
117 100
82 58.5 45.4 68.2
119 33.2 24.7 37.1

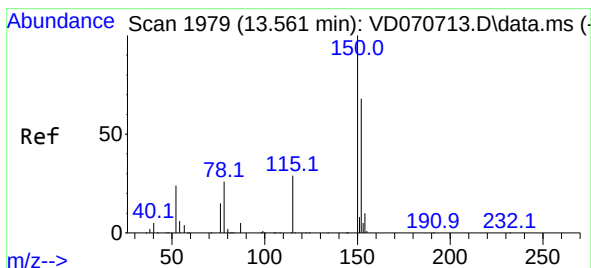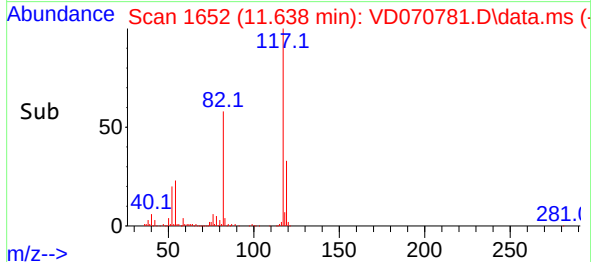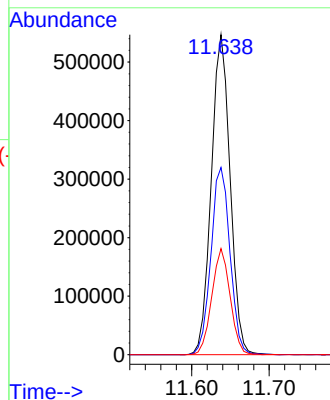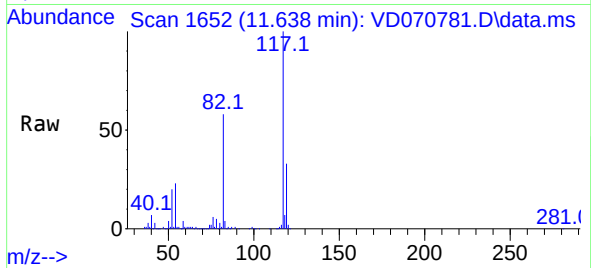

#72
1,4-Dichlorobenzene-d4
Concen: 50.00 ug/l
RT: 13.561 min Scan# 1979
Delta R.T. 0.000 min
Lab File: VD070781.D
Acq: 20 Oct 2021 17:46

Tgt Ion:152 Resp: 396364
Ion Ratio Lower Upper
152 100
115 63.2 31.9 95.7
150 159.8 0.0 350.0

