
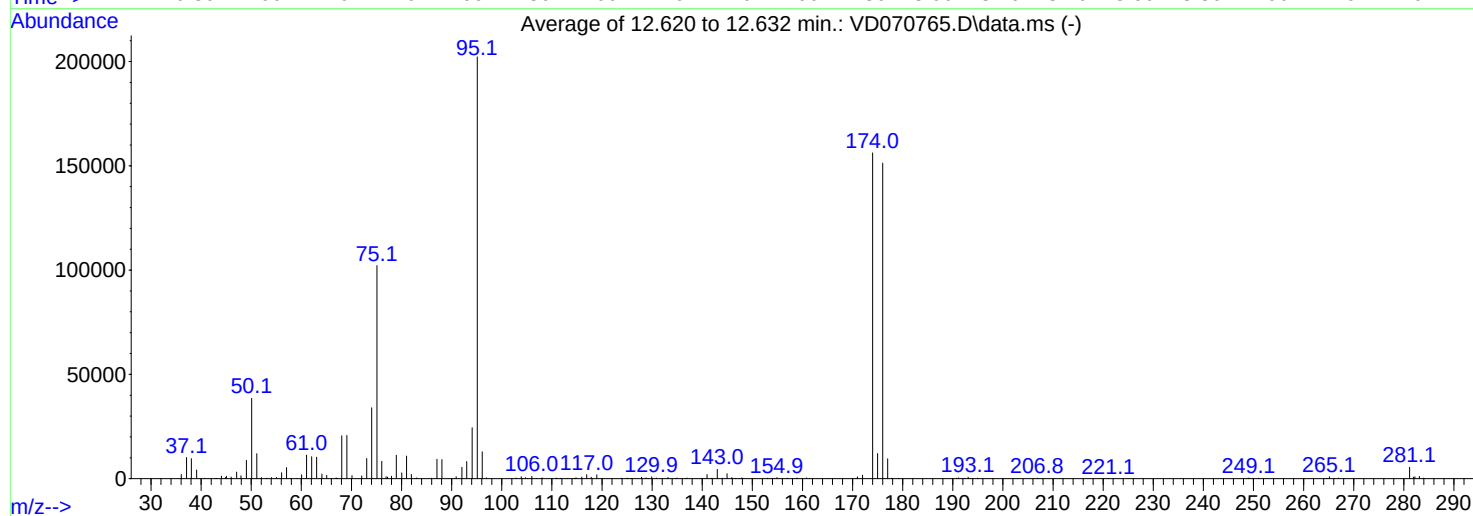


Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD102021\
 Data File : VD070765.D
 Acq On : 20 Oct 2021 09:56
 Operator : VA/SY
 Sample : BFB
 Misc : 5.00G/5.00ml/MSVOA_D/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_D
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D101521S.M
 Title : SW846 8260
 Last Update : Mon Oct 18 08:32:03 2021

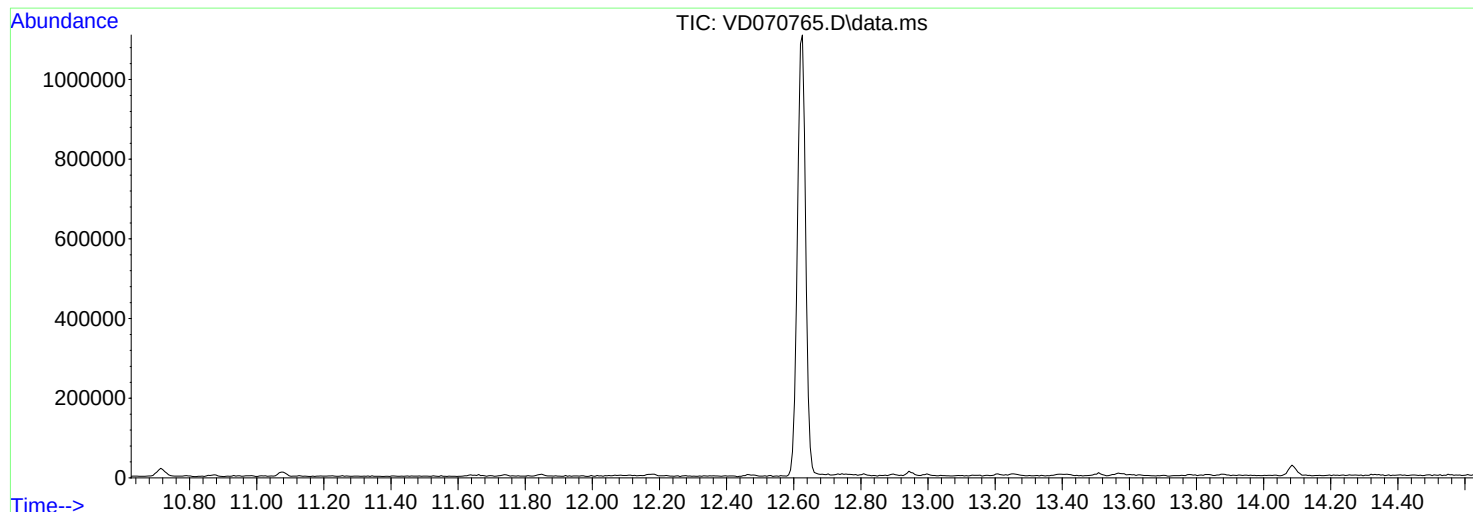

AutoFind: Scans 1819, 1820, 1821; Background Corrected with Scan 1809

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.1	38539	PASS
75	95	30	60	50.5	102176	PASS
95	95	100	100	100.0	202261	PASS
96	95	5	9	6.4	12894	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	100	77.2	156181	PASS
175	174	5	9	7.7	12039	PASS
176	174	95	101	96.9	151275	PASS
177	176	5	9	6.3	9508	PASS