

Data Path : Z:\VOASRV\HPCHEM1\MSVOA D\DATA\VD102120\
 Data File : VD067344.D
 Acq On : 21 Oct 2020 13:36
 Operator : VA/SY
 Sample : L4468-01
 Misc : 6.29G/5.00ml/MSVOA D/SOIL
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_D
 ClientSampleId :
 72-11977

Quant Time: Oct 22 00:43:13 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_D\METHOD\82D101320S.M
 Quant Title : SW846 8260
 QLast Update : Mon Oct 19 19:13:29 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	7.98	168	341572	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	8.87	114	565007	50.00	ug/l	0.00
63) Chlorobenzene-d5	11.65	117	550216	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.58	152	272904	50.00	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.34	65	184925	54.04	ug/l	0.00
Spiked Amount	50.000		Recovery	=	108.08%	
35) Dibromofluoromethane	7.92	113	186113	49.50	ug/l	0.00
Spiked Amount	50.000		Recovery	=	99.00%	
50) Toluene-d8	10.34	98	662876	48.71	ug/l	0.00
Spiked Amount	50.000		Recovery	=	97.42%	
62) 4-Bromofluorobenzene	12.64	95	247619	52.33	ug/l	0.00
Spiked Amount	50.000		Recovery	=	104.66%	


Target Compounds	Qvalue
------------------	--------


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA D\DATA\VD102120\
Data File : VD067344.D
Acq On : 21 Oct 2020 13:36
Operator : VA/SY
Sample : L4468-01
Misc : 6.29G/5.00ml/MSVOA D/SOIL
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
72-11977

Quant Time: Oct 22 00:43:13 2020
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_D\METHOD\82D101320S.M
Quant Title : SW846 8260
QLast Update : Mon Oct 19 19:13:29 2020
Response via : Initial Calibration

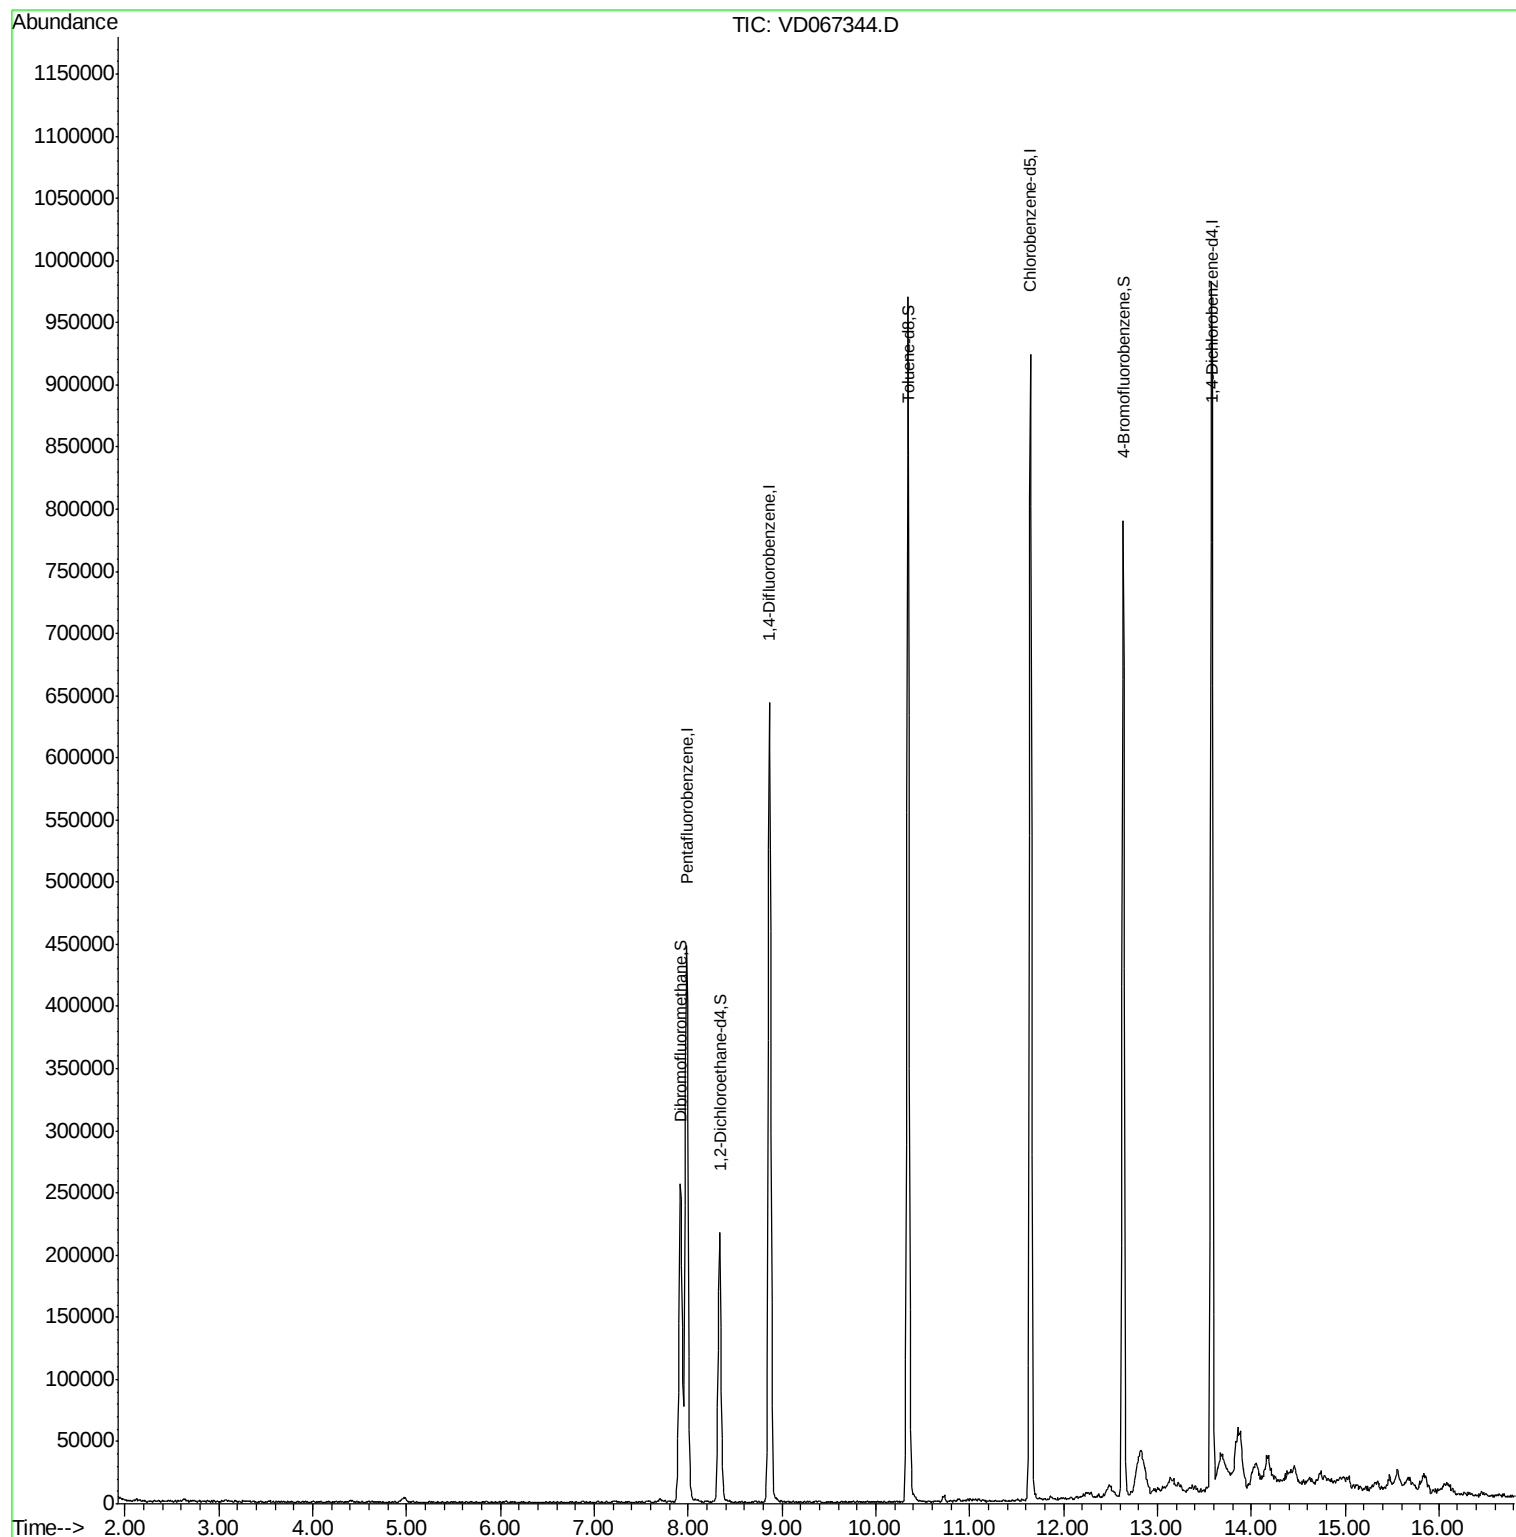

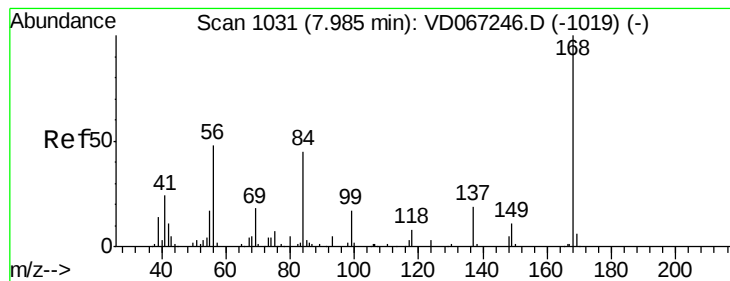

#1

Pentafluorobenzene

Concen: 50.000 ug/l

RT: 7.98 min Scan# 1031

Delta R.T. 0.00 min

Lab File: VD067344.D

Acq: 21 Oct 2020 13:36

Instrument :

MSVOA_D

ClientSampleId :


72-11977

Tot Ion:168 Resp: 341572

Ion Ratio Lower Upper

168 100

99 59.3 45.9 68.9

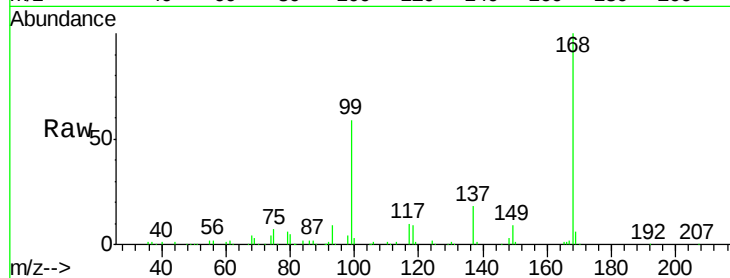

Abundance Ion 167.90 (167.60 to 168.60): V

Ion 98.90 (98.60 to 99.60): VDC

7.98

150000



100000

50000

0

Time-->

7.90 8.00 8.10

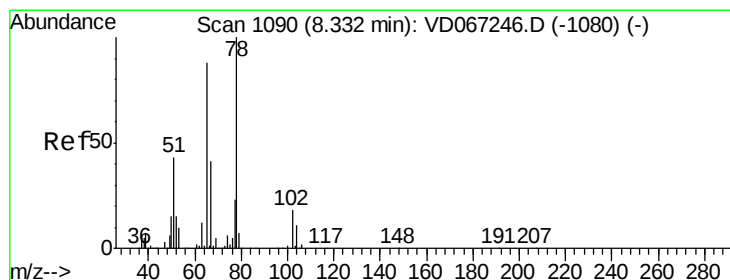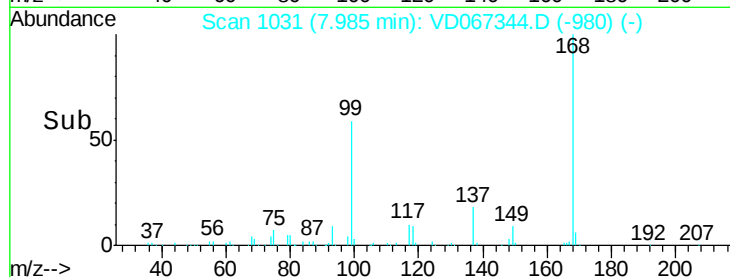

#33

1,2-Dichloroethane-d4

Concen: 54.039 ug/l

RT: 8.34 min Scan# 1091

Delta R.T. 0.01 min

Lab File: VD067344.D


Acq: 21 Oct 2020 13:36

Tgt Ion: 65 Resp: 184925

Ion Ratio Lower Upper

65 100

67 49.8 0.0 103.8

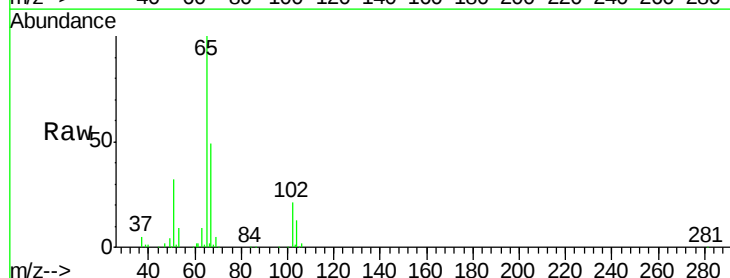

Abundance Ion 64.90 (64.60 to 65.60): VDC

Ion 66.90 (66.60 to 67.60): VDC

8.34

80000

60000


40000


20000

0

Time-->

8.20 8.30 8.40

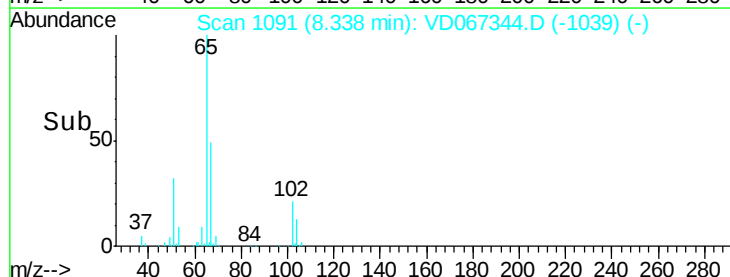


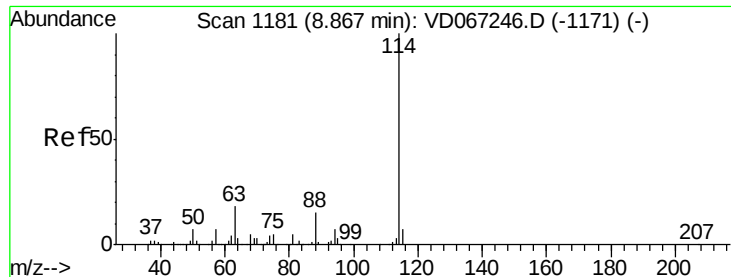


#34
 1,4-Difluorobenzene
 Concen: 50.000 ug/l
 RT: 8.87 min Scan# 1181
 Delta R.T. 0.00 min
 Lab File: VD067344.D
 Acq: 21 Oct 2020 13:36

Instrument :
 MSVOA_D
 ClientSampleId :
 72-11977



Tot Ion	Ratio	Lower	Upper
114	100		
63	17.7	0.0	35.0
88	16.2	0.0	30.6

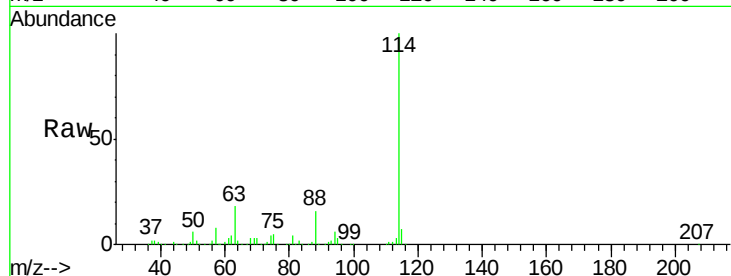

Abundance Ion 113.90 (113.60 to 114.60): V
 Ion 63.00 (62.70 to 63.70): V
 Ion 87.90 (87.60 to 88.60): V

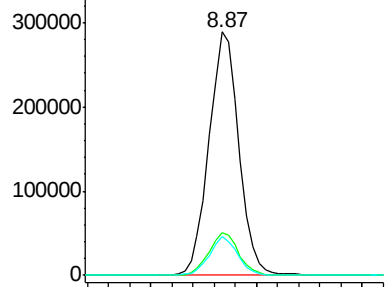


Time-->

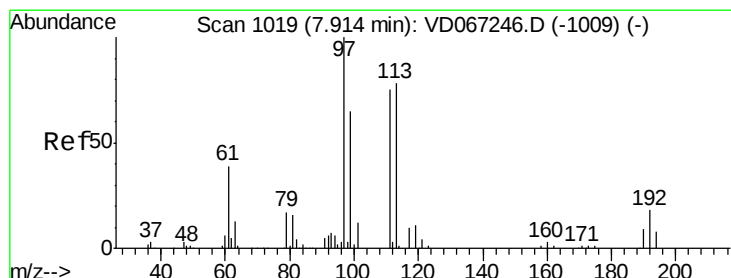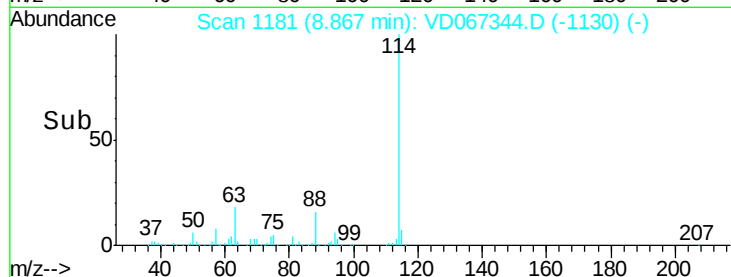


#35
 Dibromofluoromethane
 Concen: 49.496 ug/l
 RT: 7.92 min Scan# 1020
 Delta R.T. 0.01 min
 Lab File: VD067344.D
 Acq: 21 Oct 2020 13:36


Tgt Ion	Ratio	Lower	Upper
113	100		
111	101.0	81.6	122.4
192	20.4	17.0	25.4

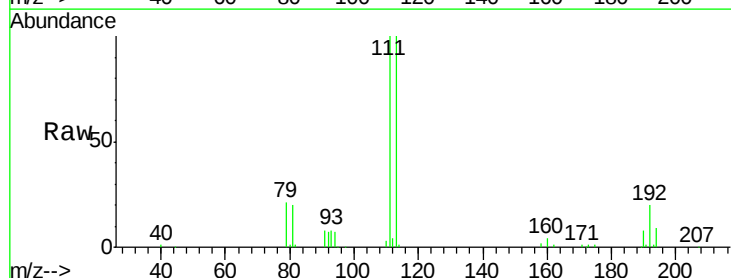


Abundance Ion 112.80 (112.50 to 113.50): V
 Ion 110.80 (110.50 to 111.50): V
 Ion 191.70 (191.40 to 192.40): V

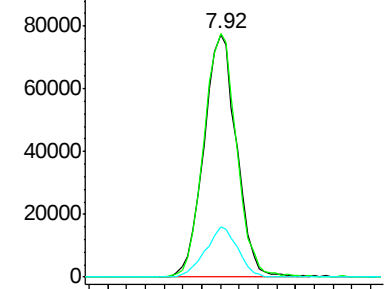

Time-->

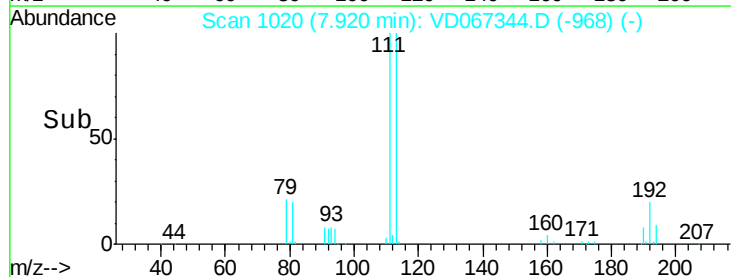

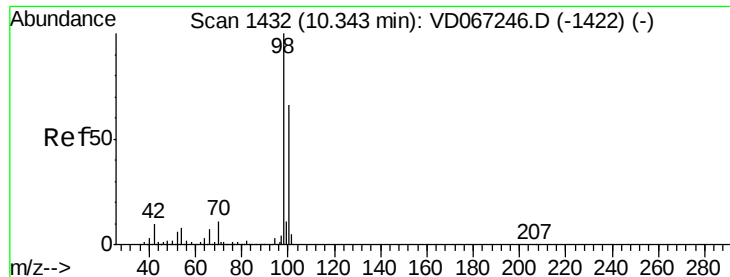

#50

Toluene-d8

Concen: 48.714 ug/l

RT: 10.34 min Scan# 1432

Delta R.T. 0.00 min

Lab File: VD067344.D

Acq: 21 Oct 2020 13:36

Instrument :

MSVOA_D

ClientSampleId :


72-11977

Tot Ion: 98 Resp: 662876

Ion Ratio Lower Upper

98 100

100 66.6 53.1 79.7

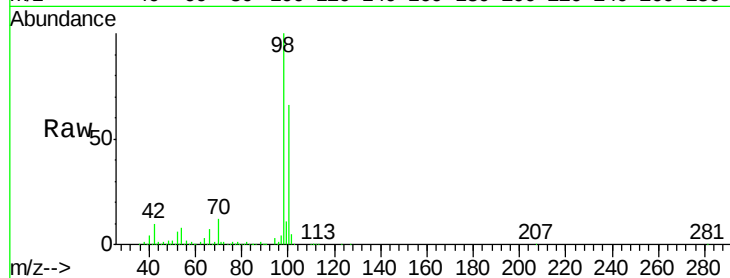

Abundance Ion 98.00 (97.70 to 98.70): VD067246.D (-1422) (-)

Ion 100.00 (99.70 to 100.70): VD067246.D (-1422) (-)

10.34

400000



300000

200000

100000

0

Time-->

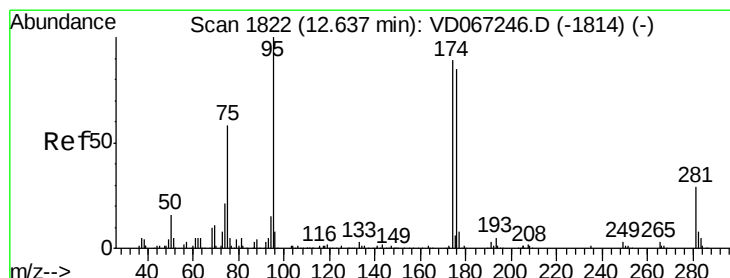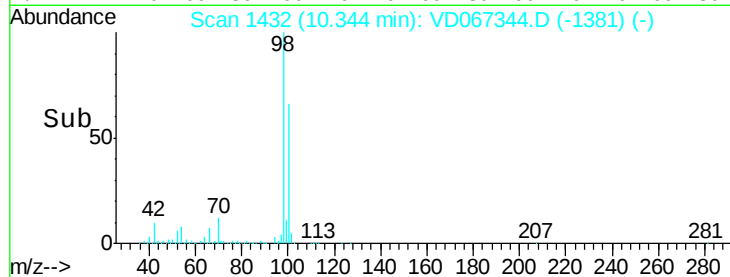

#62

4-Bromofluorobenzene

Concen: 52.333 ug/l

RT: 12.64 min Scan# 1822

Delta R.T. 0.00 min

Lab File: VD067344.D

Acq: 21 Oct 2020 13:36


Tgt Ion: 95 Resp: 247619

Ion Ratio Lower Upper

95 100

174 88.0 0.0 175.2

176 84.6 0.0 168.6

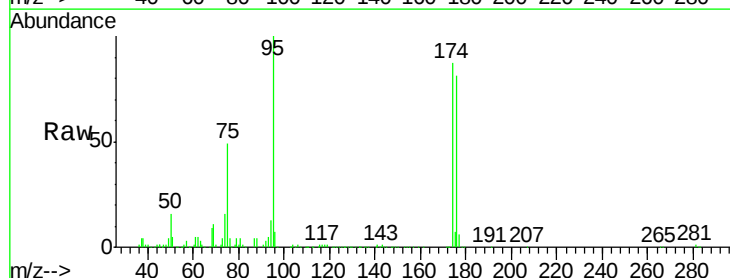

Abundance Ion 94.90 (94.60 to 95.60): VD067246.D (-1814) (-)

Ion 173.80 (173.50 to 174.50): VD067246.D (-1814) (-)

Ion 175.80 (175.50 to 176.50): VD067246.D (-1814) (-)

12.64

200000


150000


100000

50000

0

Time-->

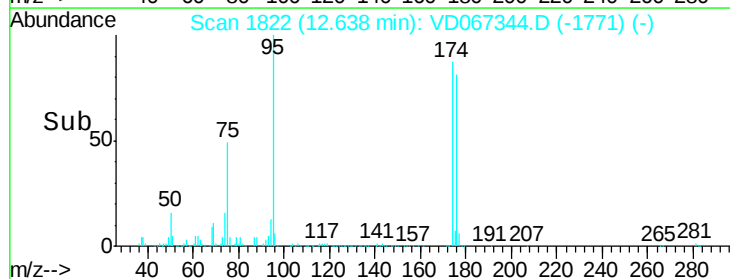


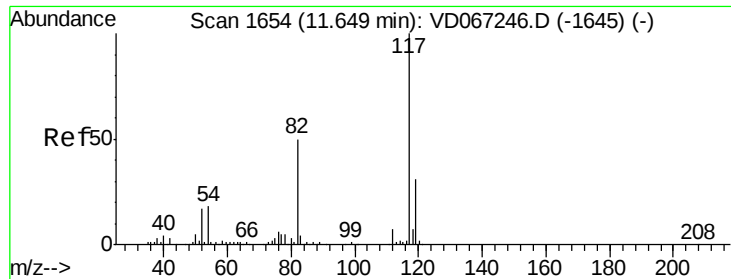




#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.65 min Scan# 1654
Delta R.T. 0.00 min
Lab File: VD067344.D
Acq: 21 Oct 2020 13:36

Instrument :
MSVOA_D
ClientSampleId :
72-11977

Tot Ion:117 Resp: 550216
Ion Ratio Lower Upper
117 100
82 51.4 39.9 59.9
119 33.9 24.9 37.3

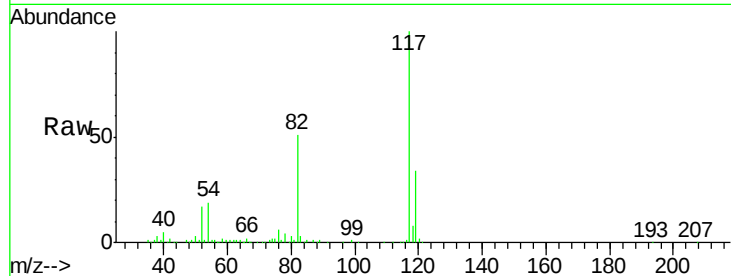


Abundance Ion 116.90 (116.60 to 117.60): V
Ion 82.00 (81.70 to 82.70): V
Ion 118.90 (118.60 to 119.60): V

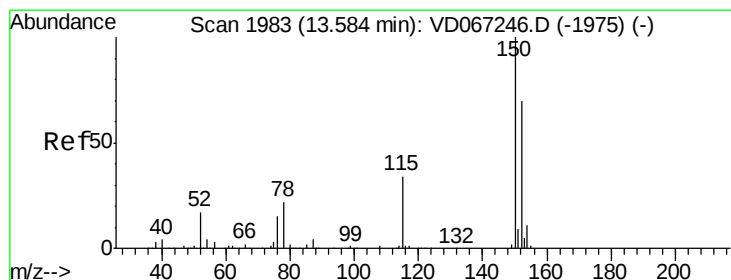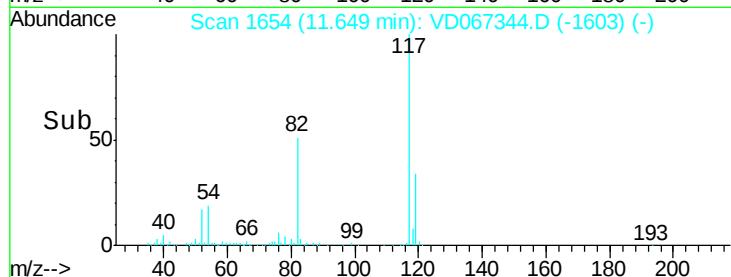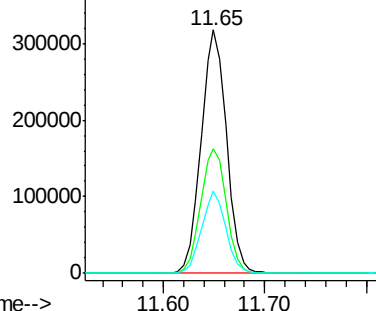

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.58 min Scan# 1982
Delta R.T. -0.01 min
Lab File: VD067344.D
Acq: 21 Oct 2020 13:36

Tgt Ion:152 Resp: 272904
Ion Ratio Lower Upper
152 100
115 60.5 29.3 87.9
150 156.9 0.0 339.0

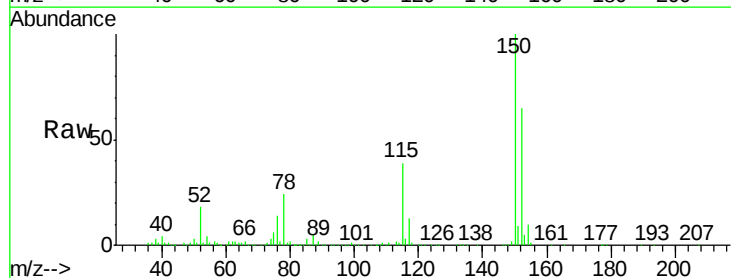

Abundance Ion 151.90 (151.60 to 152.60): V
Ion 114.90 (114.60 to 115.60): V
Ion 149.90 (149.60 to 150.60): V

