


Data Path : Z:\voasrv\HPCHEM1\MSVOA D\Data\VD102120\
Data File : VD067336.D
Acq On : 21 Oct 2020 09:36
Operator : VA/SY
Sample : BFB
Misc : 5.00G/5.00ml/MSVOA D/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_D\METHOD\82D101320S.M
Title : SW846 8260
Last Update : Mon Oct 19 19:13:29 2020

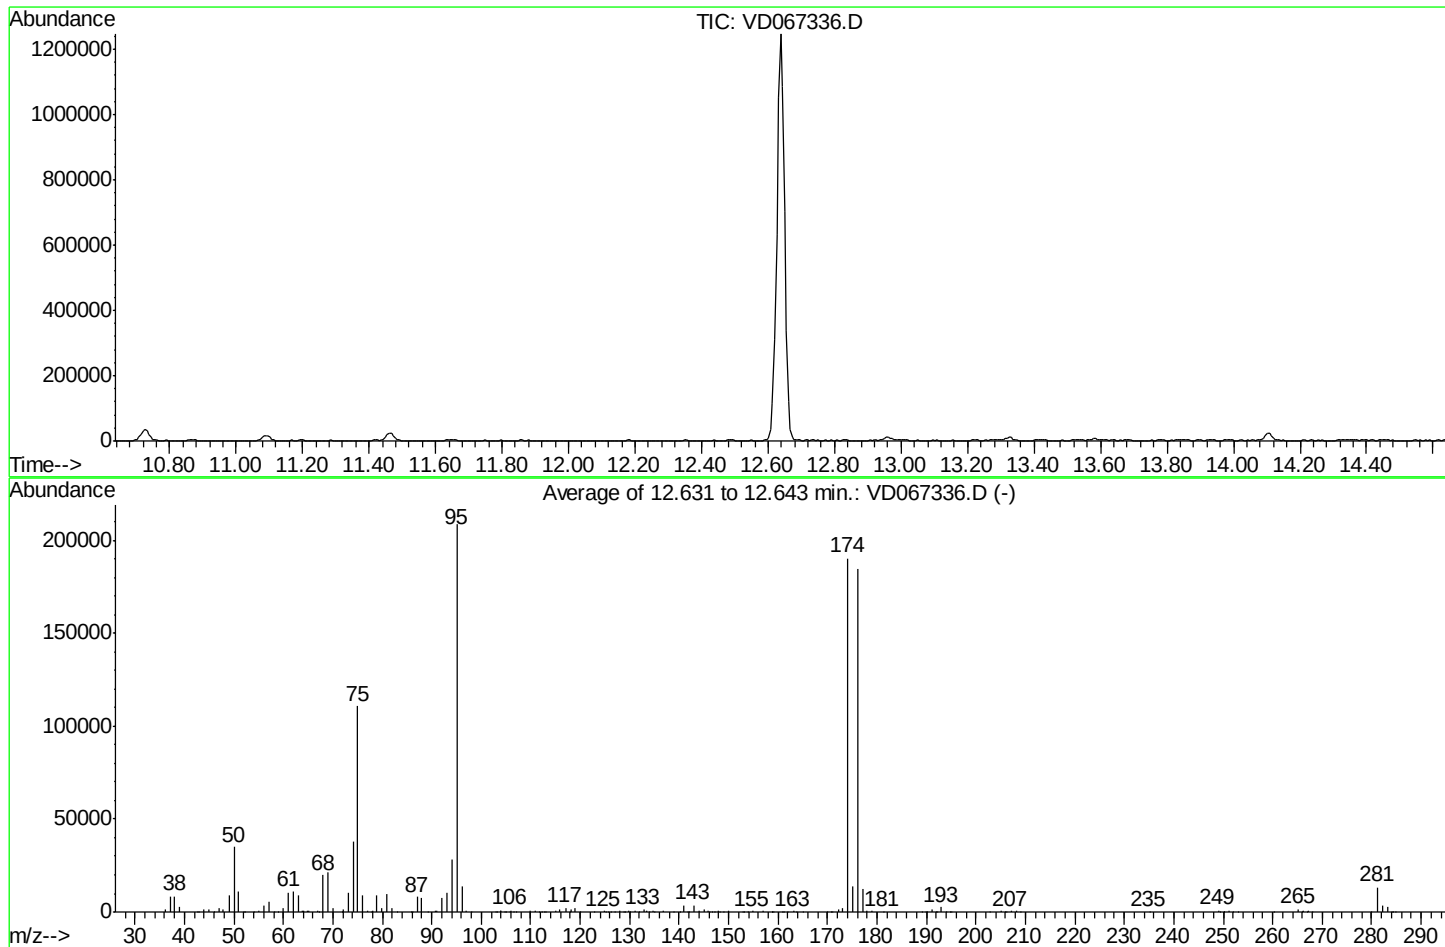

AutoFind: Scans 1821, 1822, 1823; Background Corrected with Scan 1811

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.8	35090	PASS
75	95	30	60	53.1	110856	PASS
95	95	100	100	100.0	208682	PASS
96	95	5	9	6.6	13744	PASS
173	174	0.00	2	1.1	2153	PASS
174	95	50	100	91.2	190400	PASS
175	174	5	9	7.2	13675	PASS
176	174	95	101	97.1	184832	PASS
177	176	5	9	6.8	12650	PASS