


Data Path : Z:\VOASRV\HPCHEM1\MSVOA D\DATA\VD102918\
Data File : VD060226.D
Acq On : 29 Oct 2018 13:23
Operator : VA/AP
Sample : BFB
Misc : 5.00µl/5ml/MSVOA D/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_D\METHOD\82D100118S.M
Title : SW846 8260
Last Update : Tue Oct 02 06:56:35 2018

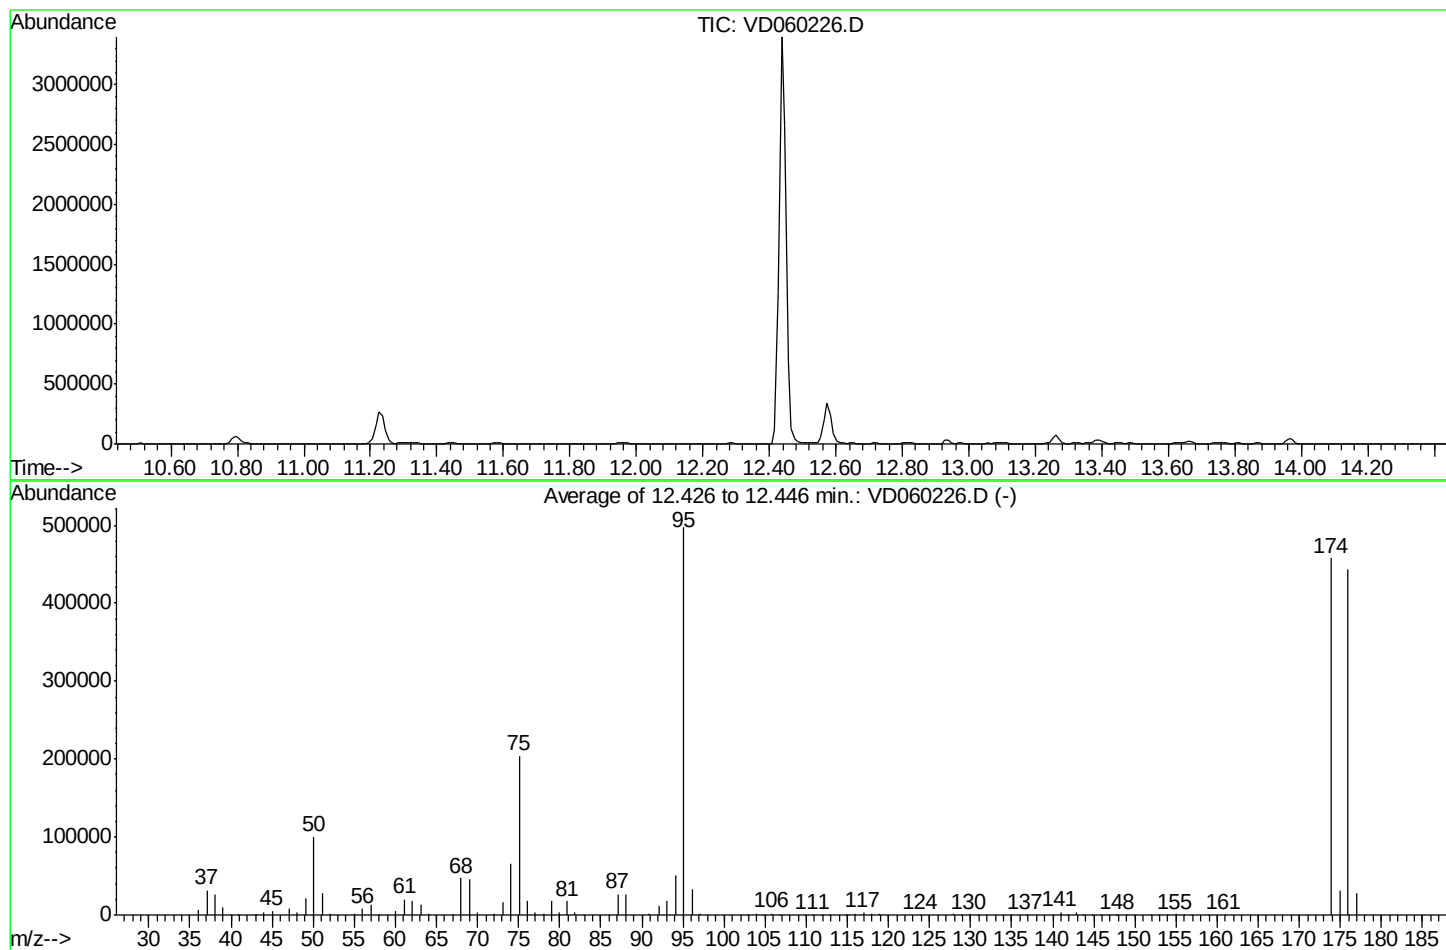

AutoFind: Scans 1108, 1109, 1110; Background Corrected with Scan 1104

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.2	100392	PASS
75	95	30	60	41.0	203768	PASS
95	95	100	100	100.0	497322	PASS
96	95	5	9	6.6	33053	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	100	92.1	457834	PASS
175	174	5	9	6.9	31643	PASS
176	174	95	101	96.7	442794	PASS
177	176	5	9	6.5	28581	PASS