


Data Path : Z:\VOASRV\HPCHEM1\MSVOA_D\DATA\VD103119\
 Data File : VD064125.D
 Acq On : 31 Oct 2019 10:40
 Operator : VA/SY
 Sample : BFB
 Misc : 5.00G/5.00ml/MSVOA_D/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_D
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_D\METHOD\82D102919S.M
 Title : SW846 8260
 Last Update : Wed Oct 30 08:00:10 2019

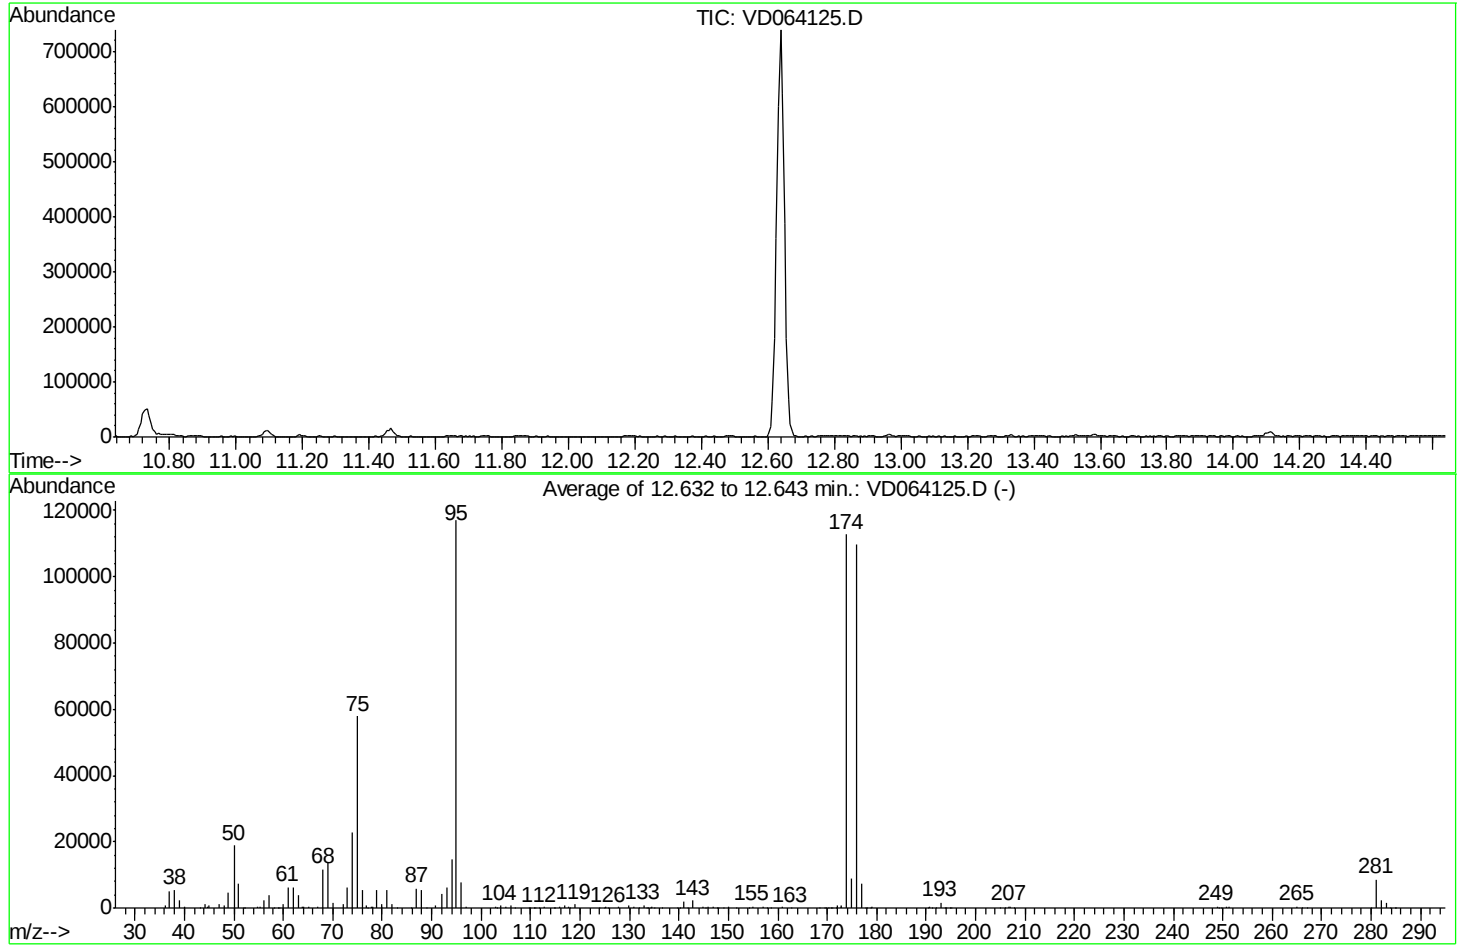

AutoFind: Scans 1821, 1822, 1823; Background Corrected with Scan 1813

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.2	18901	PASS
75	95	30	60	49.5	57952	PASS
95	95	100	100	100.0	117029	PASS
96	95	5	9	6.7	7787	PASS
173	174	0.00	2	0.8	903	PASS
174	95	50	100	96.3	112725	PASS
175	174	5	9	7.8	8758	PASS
176	174	95	101	97.3	109714	PASS
177	176	5	9	6.6	7253	PASS