

Data Path : Z:\VOASRV\HPCHEM1\MSVOA D\DATA\VD110420\
 Data File : VD067526.D
 Acq On : 04 Nov 2020 17:55
 Operator : VA/SY
 Sample : L4625-14
 Misc : 6.67G/5.00ml/MSVOA D/SOIL
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_D
 ClientSampleId :
 CONTAINER-002-2B

Quant Time: Nov 05 01:37:07 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_D\METHOD\82D110320S.M
 Quant Title : SW846 8260
 QLast Update : Wed Nov 04 00:56:28 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	7.98	168	279070	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	8.87	114	466286	50.00	ug/l	0.00
63) Chlorobenzene-d5	11.65	117	447533	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.58	152	197932	50.00	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.33	65	149731	61.36	ug/l	0.00
Spiked Amount	50.000		Recovery	=	122.72%	
35) Dibromofluoromethane	7.92	113	151521	53.93	ug/l	0.00
Spiked Amount	50.000		Recovery	=	107.86%	
50) Toluene-d8	10.34	98	542232	54.92	ug/l	0.00
Spiked Amount	50.000		Recovery	=	109.84%	
62) 4-Bromofluorobenzene	12.64	95	191125	56.07	ug/l	0.00
Spiked Amount	50.000		Recovery	=	112.14%	


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA D\DATA\VD110420\
Data File : VD067526.D
Acq On : 04 Nov 2020 17:55
Operator : VA/SY
Sample : L4625-14
Misc : 6.67G/5.00ml/MSVOA D/SOIL
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
CONTAINER-002-2B

Quant Time: Nov 05 01:37:07 2020
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_D\METHOD\82D110320S.M
Quant Title : SW846 8260
QLast Update : Wed Nov 04 00:56:28 2020
Response via : Initial Calibration

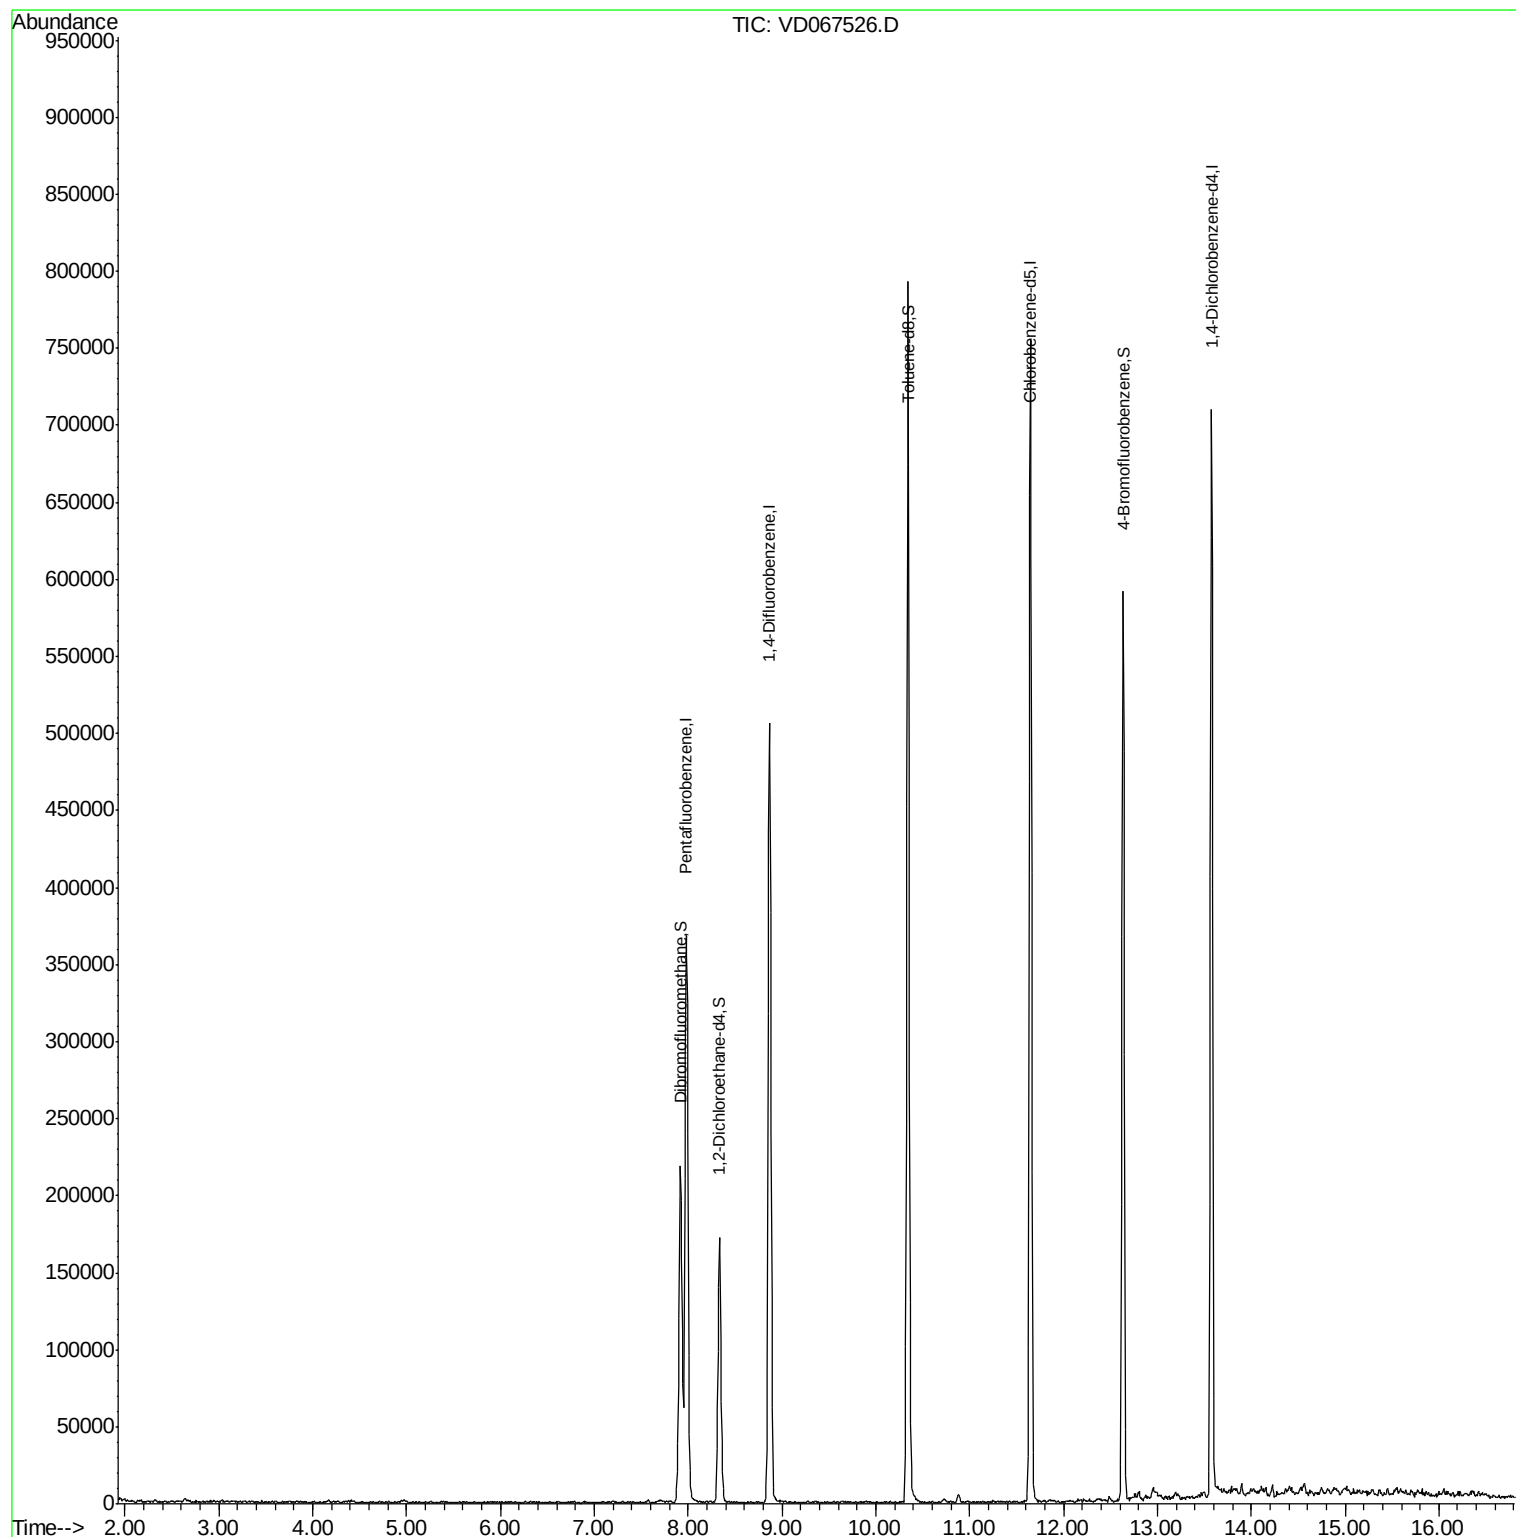

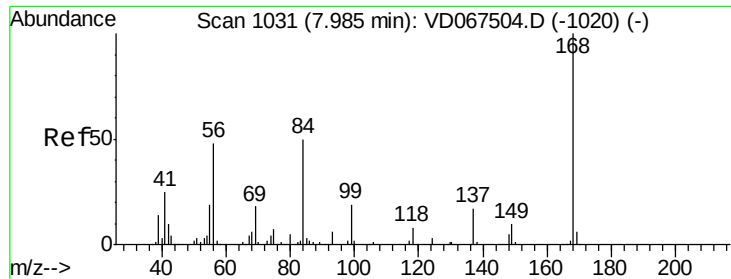

#1

Pentafluorobenzene

Concen: 50.000 ug/l

RT: 7.98 min Scan# 1030

Delta R.T. -0.01 min

Lab File: VD067526.D

Acq: 04 Nov 2020 17:55

Instrument :

MSVOA_D

ClientSampleId :


CONTAINER-002-2B

Tot Ion:168 Resp: 279070

Ion Ratio Lower Upper

168 100

99 55.5 45.0 67.6

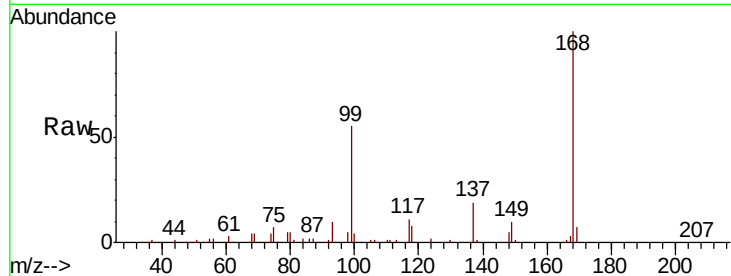

Abundance Ion 167.90 (167.60 to 168.60): V

Ion 98.90 (98.60 to 99.60): VDC



7.98

100000

50000

0

Time-->

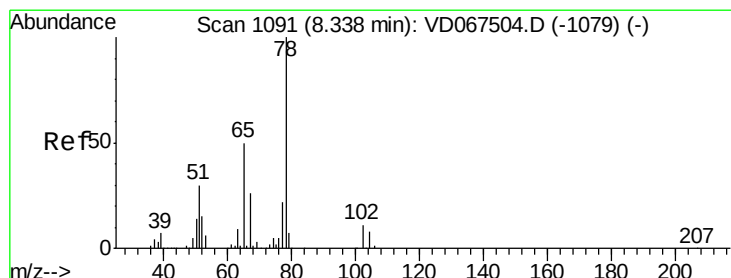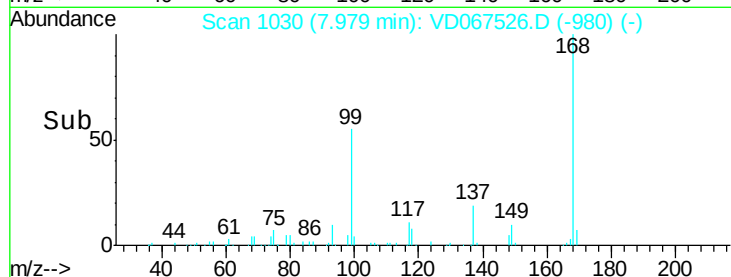

#33

1,2-Dichloroethane-d4

Concen: 61.361 ug/l

RT: 8.33 min Scan# 1090

Delta R.T. -0.01 min

Lab File: VD067526.D


Acq: 04 Nov 2020 17:55

Tgt Ion: 65 Resp: 149731

Ion Ratio Lower Upper

65 100

67 48.4 0.0 99.4

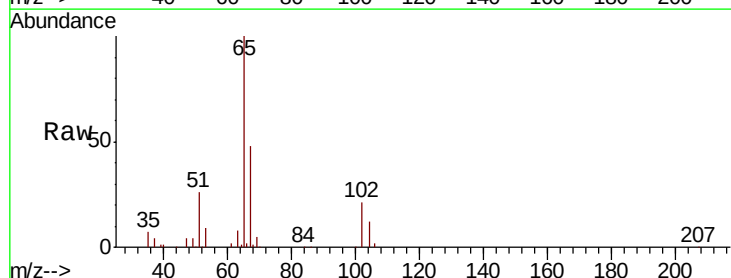

Abundance Ion 64.90 (64.60 to 65.60): VDC

Ion 66.90 (66.60 to 67.60): VDC

8.33

80000


60000


40000

20000

0

Time-->

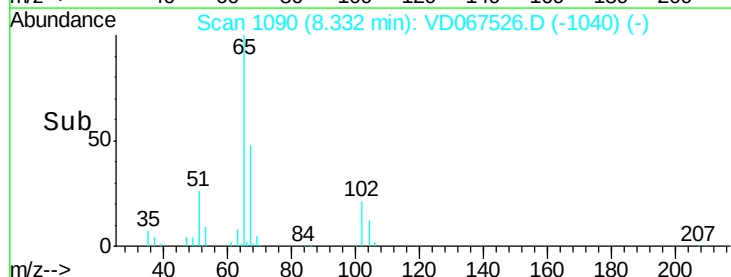


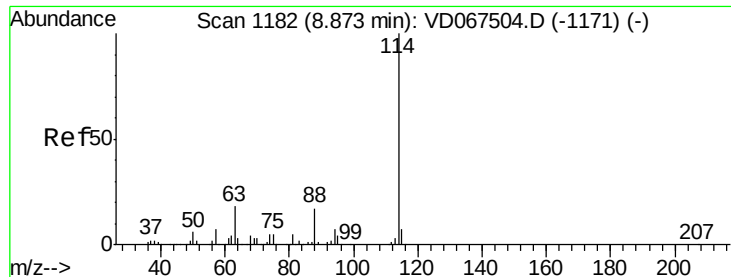




#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 8.87 min Scan# 1181
Delta R.T. -0.01 min
Lab File: VD067526.D
Acq: 04 Nov 2020 17:55

Instrument :
MSVOA_D
ClientSampleId :
CONTAINER-002-2B

Tot Ion	Ratio	Lower	Upper
114	100		
63	17.4	0.0	35.0
88	15.7	0.0	33.0

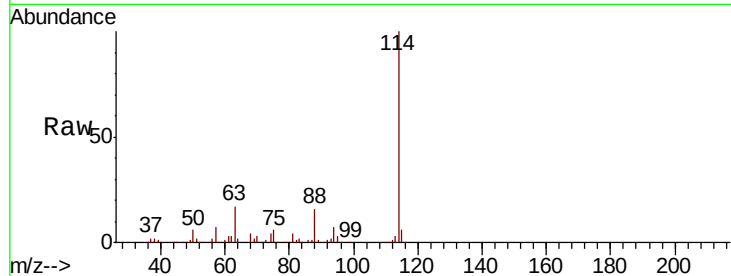


Abundance Ion 113.90 (113.60 to 114.60): V
Ion 63.00 (62.70 to 63.70): V
Ion 87.90 (87.60 to 88.60): V

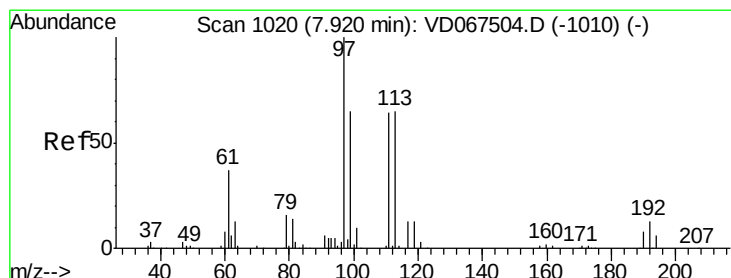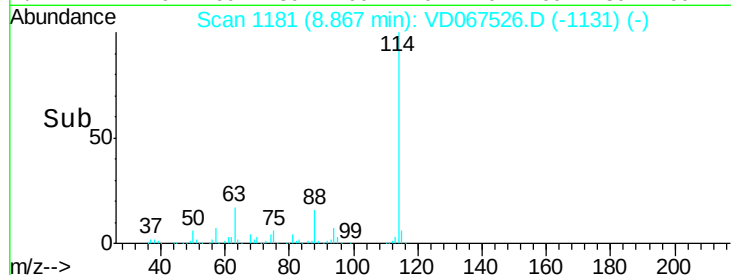
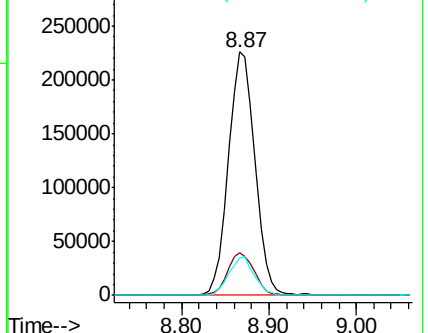



#35
Dibromofluoromethane
Concen: 53.934 ug/l
RT: 7.92 min Scan# 1020
Delta R.T. -0.00 min
Lab File: VD067526.D
Acq: 04 Nov 2020 17:55

Tgt Ion	Ratio	Lower	Upper
113	100		
111	100.5	80.0	120.0
192	21.0	16.3	24.5

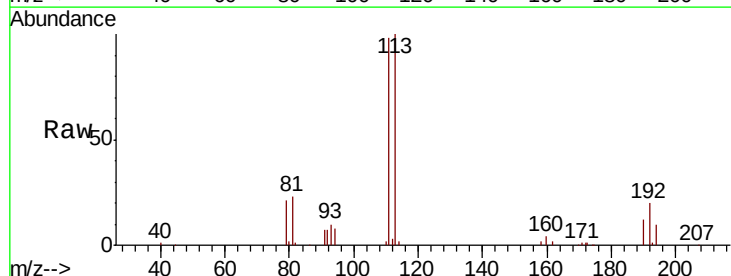

Abundance Ion 112.80 (112.50 to 113.50): V
Ion 110.80 (110.50 to 111.50): V
Ion 191.70 (191.40 to 192.40): V



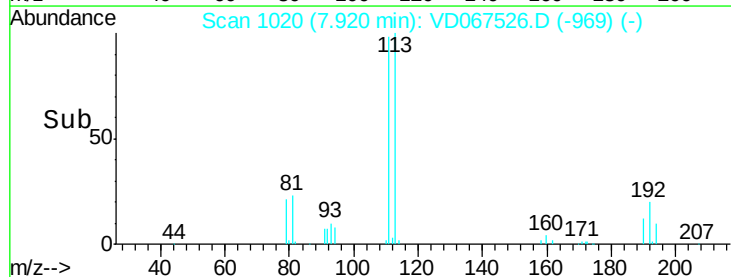
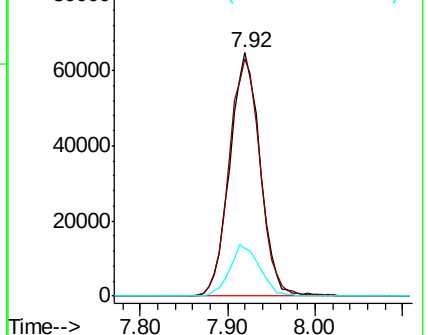


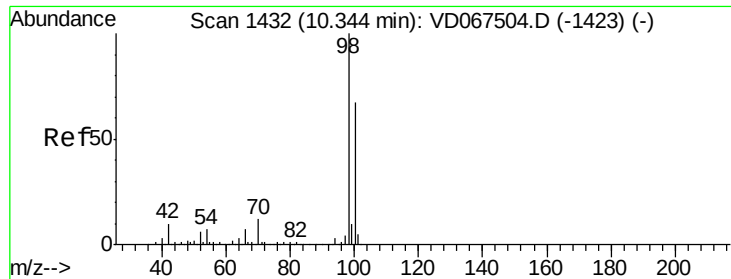

#50
Toluene-d8
Concen: 54.922 ug/l
RT: 10.34 min Scan# 1432
Delta R.T. -0.00 min
Lab File: VD067526.D
Acq: 04 Nov 2020 17:55




Instrument :
MSVOA_D
ClientSampleId :
CONTAINER-002-2B


Tot Ion: 98 Resp: 542232
Ion Ratio Lower Upper
98 100
100 65.4 53.0 79.6

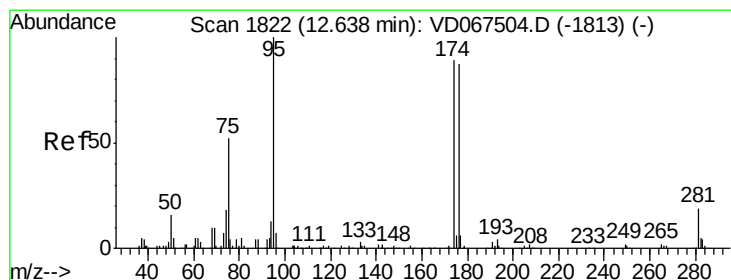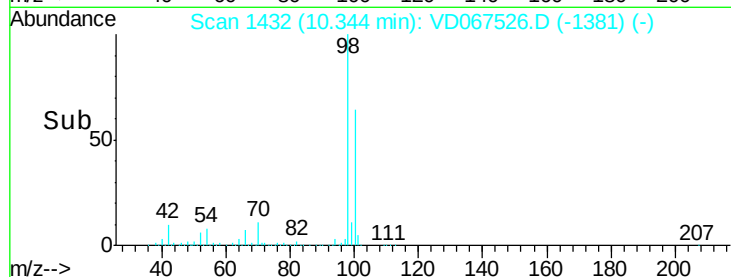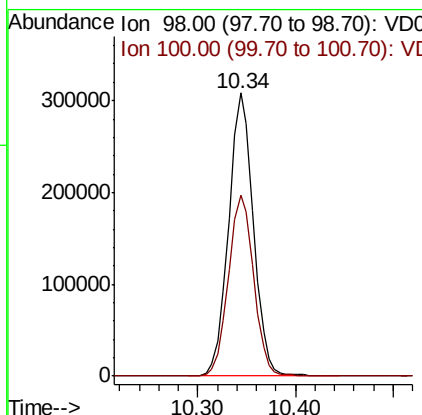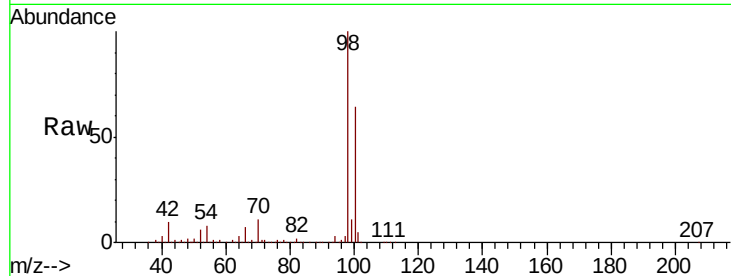

#62
4-Bromofluorobenzene
Concen: 56.073 ug/l
RT: 12.64 min Scan# 1822
Delta R.T. -0.00 min
Lab File: VD067526.D
Acq: 04 Nov 2020 17:55

Tgt Ion: 95 Resp: 191125
Ion Ratio Lower Upper
95 100
174 89.1 0.0 177.8
176 84.9 0.0 172.0


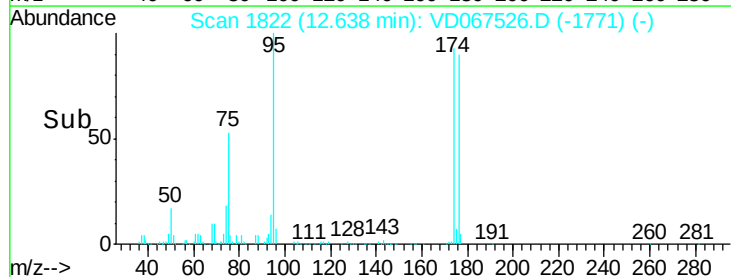
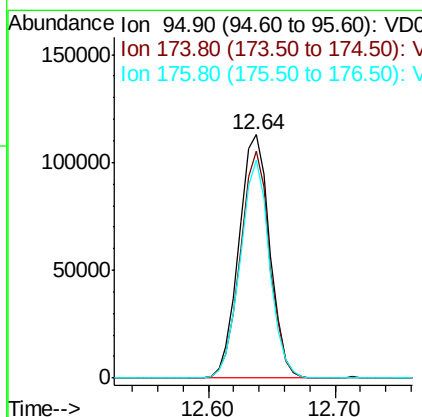
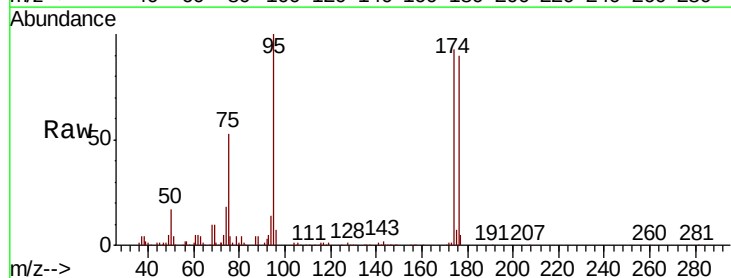


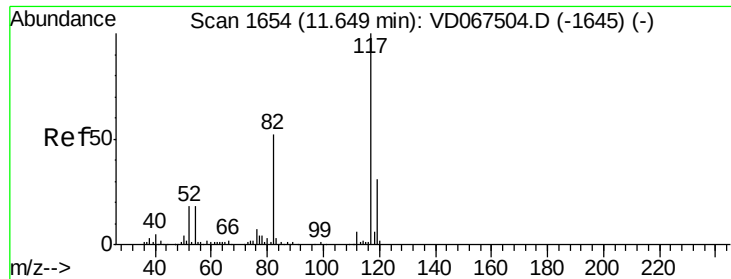

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.65 min Scan# 1654
Delta R.T. -0.00 min
Lab File: VD067526.D
Acq: 04 Nov 2020 17:55

Instrument :
MSVOA_D
ClientSampleId :
CONTAINER-002-2B

Tot Ion	Ratio	Lower	Upper
117	100		
82	48.6	41.6	62.4
119	32.1	25.1	37.7

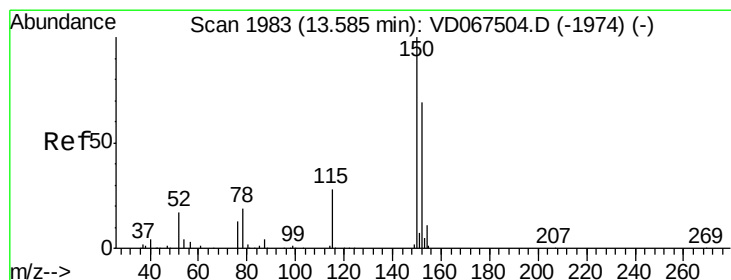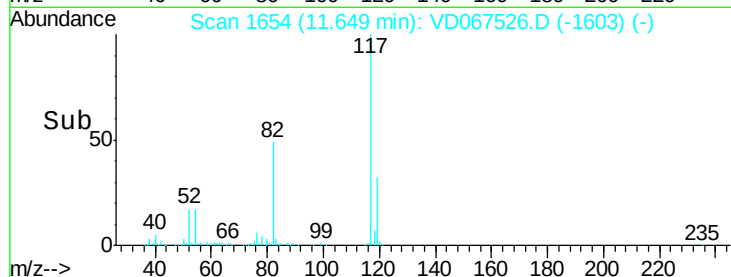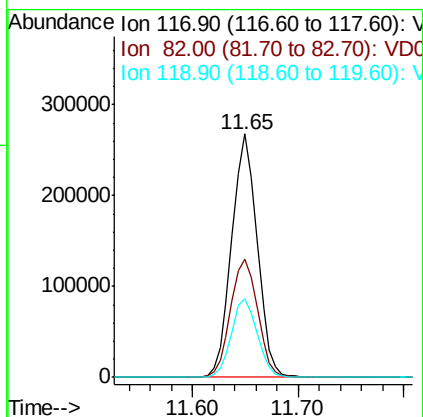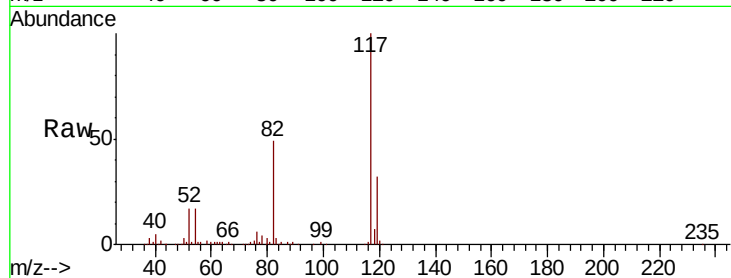

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.58 min Scan# 1982
Delta R.T. -0.01 min
Lab File: VD067526.D
Acq: 04 Nov 2020 17:55

Tgt Ion	Ratio	Lower	Upper
152	100		
115	58.8	29.3	88.0
150	156.9	0.0	338.2

