


Data Path : Z:\voasrv\HPCHEM1\MSVOA D\Data\VD110420\
 Data File : VD067508.D
 Acq On : 04 Nov 2020 09:24
 Operator : VA/SY
 Sample : BFB
 Misc : 5.00G/5.00ml/MSVOA D/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_D
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_D\METHOD\82D110320S.M
 Title : SW846 8260
 Last Update : Wed Nov 04 00:56:28 2020

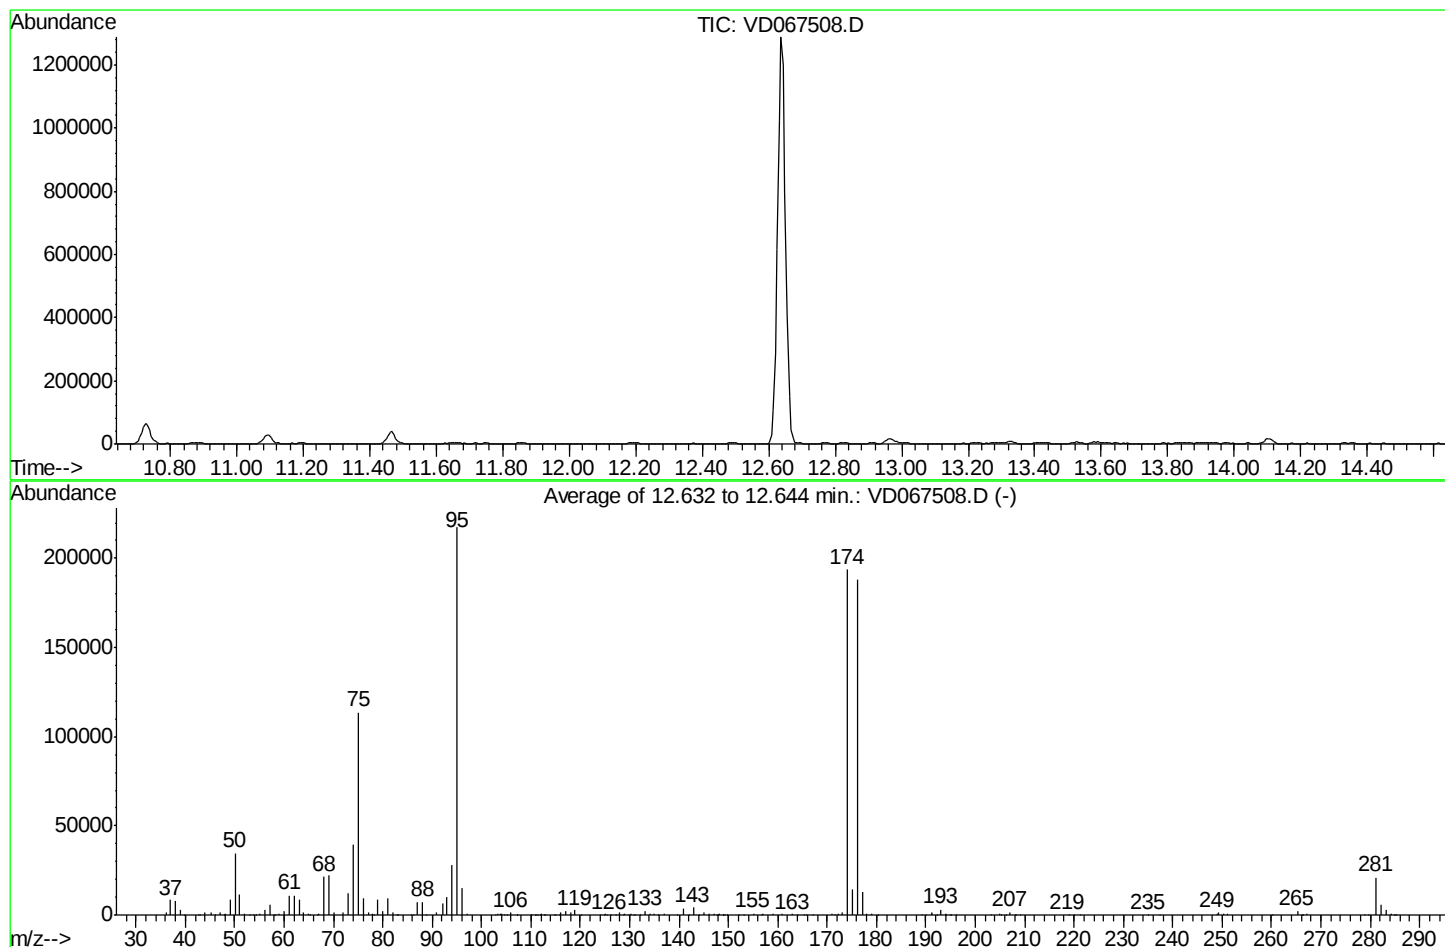

AutoFind: Scans 1821, 1822, 1823; Background Corrected with Scan 1812

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	15.9	34648	PASS
75	95	30	60	52.2	113573	PASS
95	95	100	100	100.0	217386	PASS
96	95	5	9	6.8	14789	PASS
173	174	0.00	2	0.8	1611	PASS
174	95	50	100	89.0	193493	PASS
175	174	5	9	7.3	14161	PASS
176	174	95	101	97.1	187861	PASS
177	176	5	9	6.9	12997	PASS