

Data Path : Z:\VOASRV\HPCHEM1\MSVOA D\DATA\VD110520\
 Data File : VD067538.D
 Acq On : 05 Nov 2020 13:20
 Operator : VA/SY
 Sample : L4635-01
 Misc : 5.95G/5.00ml/MSVOA D/SOIL
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_D
 ClientSampleId :
 356

Quant Time: Nov 06 00:36:40 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_D\METHOD\82D110320S.M
 Quant Title : SW846 8260
 QLast Update : Wed Nov 04 00:56:28 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	7.98	168	311266	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	8.87	114	502540	50.00	ug/l	0.00
63) Chlorobenzene-d5	11.65	117	516130	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.58	152	250986	50.00	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.33	65	160848	59.10	ug/l	0.00
Spiked Amount	50.000		Recovery	=	118.20%	
35) Dibromofluoromethane	7.91	113	163863	54.12	ug/l	0.00
Spiked Amount	50.000		Recovery	=	108.24%	
50) Toluene-d8	10.34	98	594536	55.88	ug/l	0.00
Spiked Amount	50.000		Recovery	=	111.76%	
62) 4-Bromofluorobenzene	12.64	95	226833	61.75	ug/l	0.00
Spiked Amount	50.000		Recovery	=	123.50%	


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA D\DATA\VD110520\
Data File : VD067538.D
Acq On : 05 Nov 2020 13:20
Operator : VA/SY
Sample : L4635-01
Misc : 5.95G/5.00ml/MSVOA D/SOIL
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
356

Quant Time: Nov 06 00:36:40 2020
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_D\METHOD\82D110320S.M
Quant Title : SW846 8260
QLast Update : Wed Nov 04 00:56:28 2020
Response via : Initial Calibration

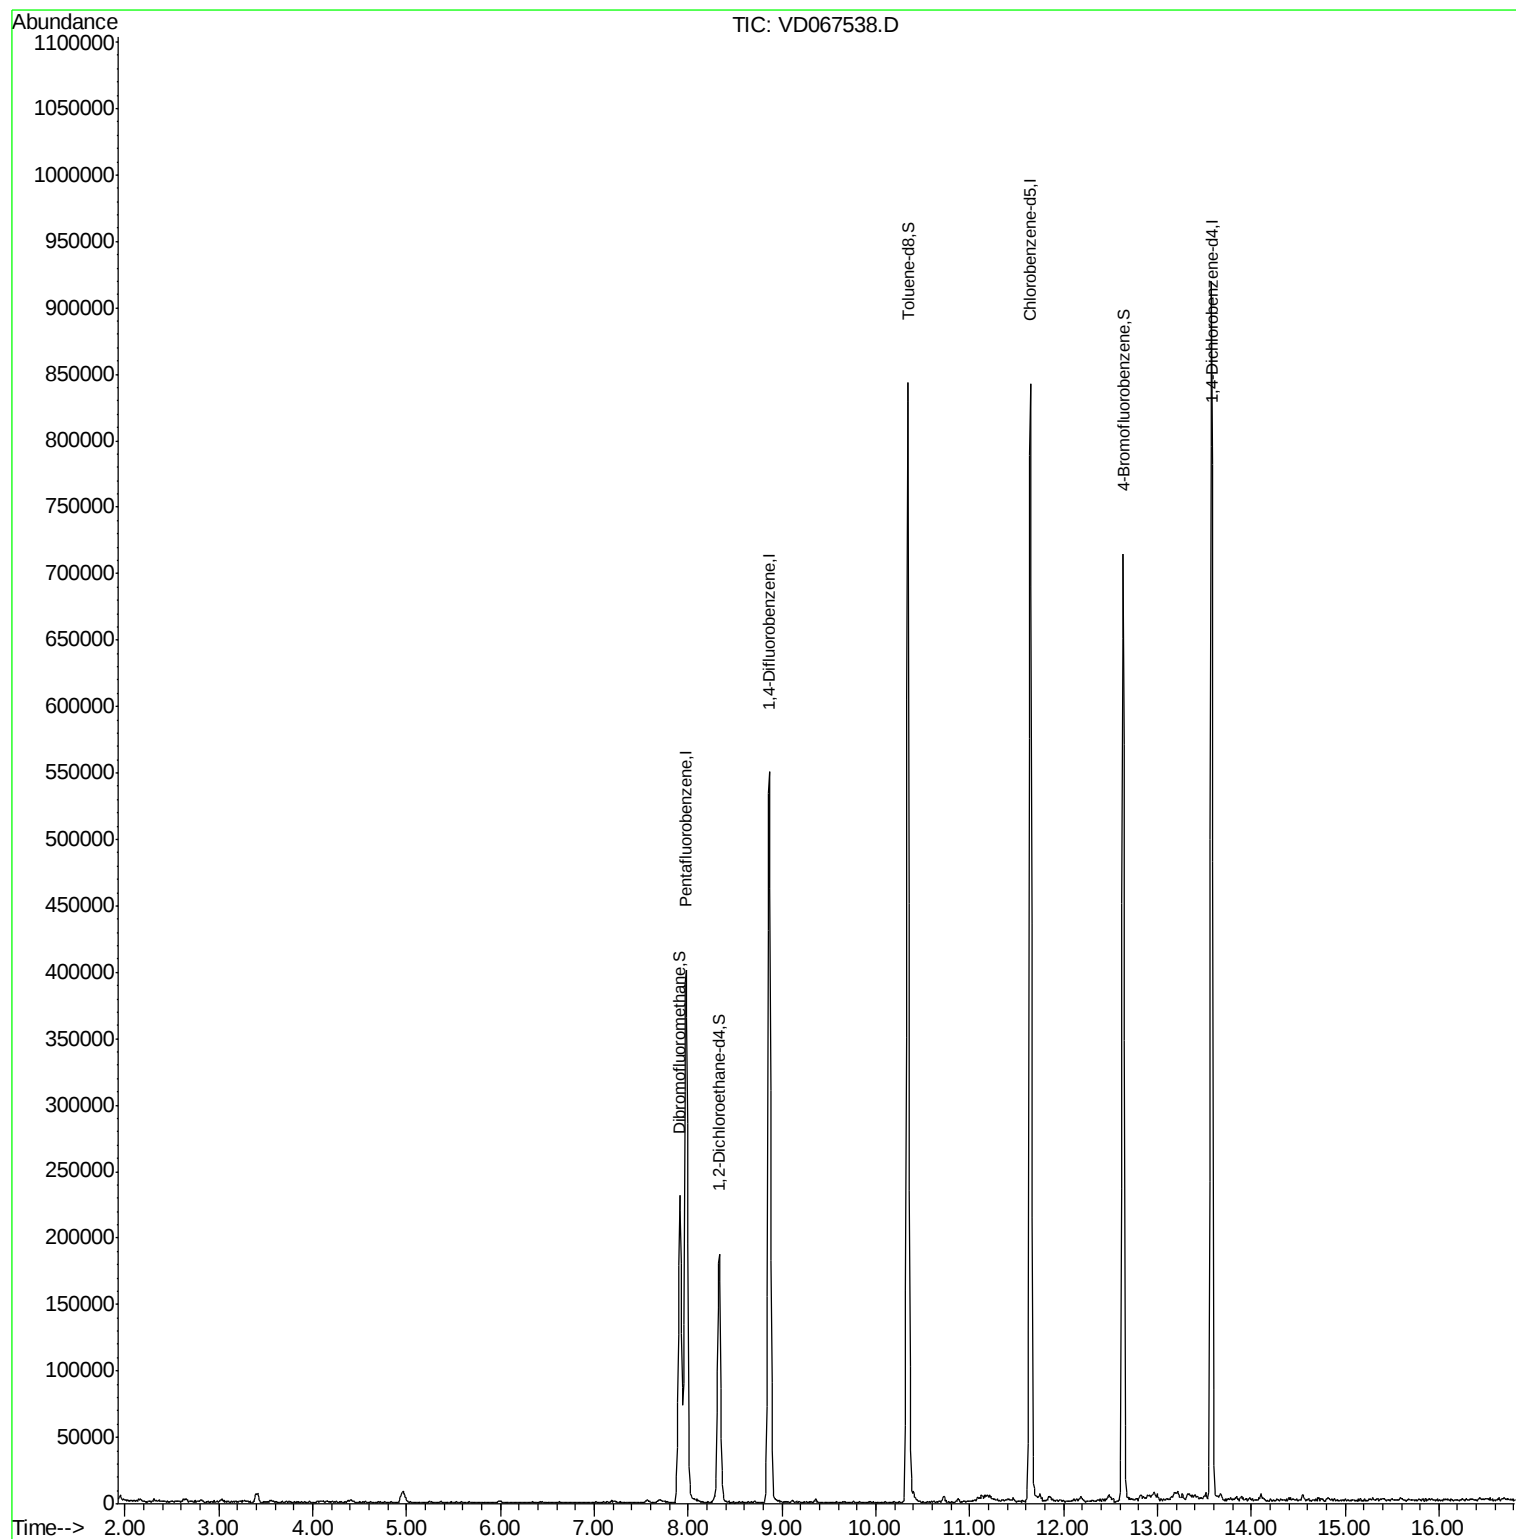

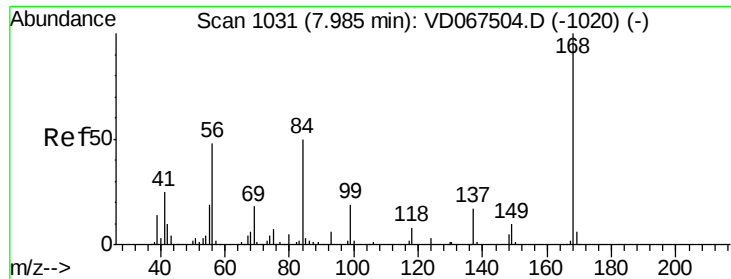

#1

Pentafluorobenzene

Concen: 50.000 ug/l

RT: 7.98 min Scan# 1030

Delta R.T. -0.01 min

Lab File: VD067538.D

Acq: 05 Nov 2020 13:20

Instrument :

MSVOA_D

ClientSampleId :


356

Tot Ion:168 Resp: 311266

Ion Ratio Lower Upper

168 100

99 53.6 45.0 67.6

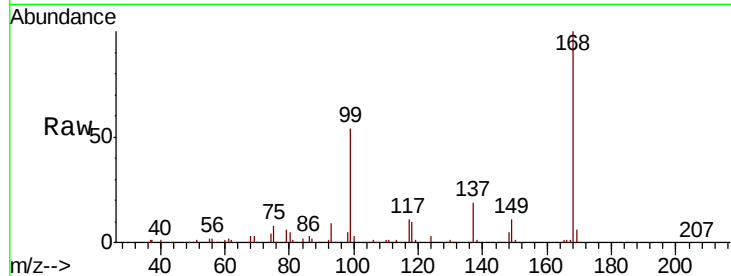

Abundance Ion 167.90 (167.60 to 168.60): V

Ion 98.90 (98.60 to 99.60): VDC

7.98



150000

100000

50000

0

Time-->

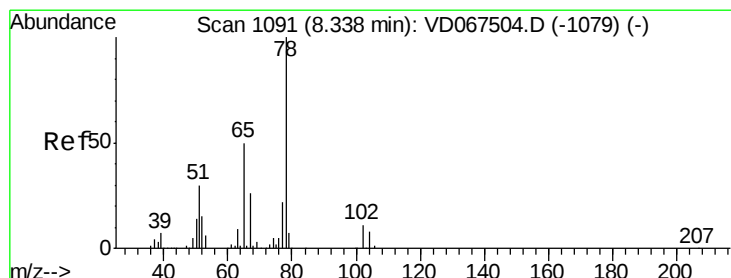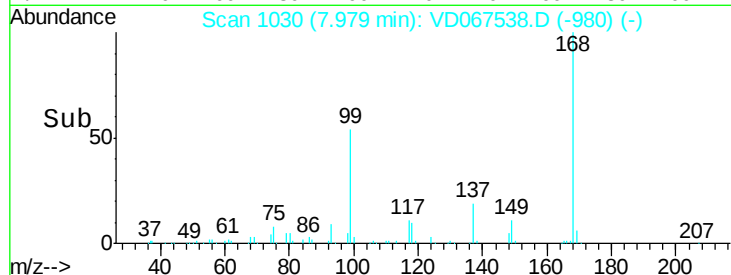

#33

1,2-Dichloroethane-d4

Concen: 59.099 ug/l

RT: 8.33 min Scan# 1090

Delta R.T. -0.01 min

Lab File: VD067538.D


Acq: 05 Nov 2020 13:20

Tgt Ion: 65 Resp: 160848

Ion Ratio Lower Upper

65 100

67 49.9 0.0 99.4

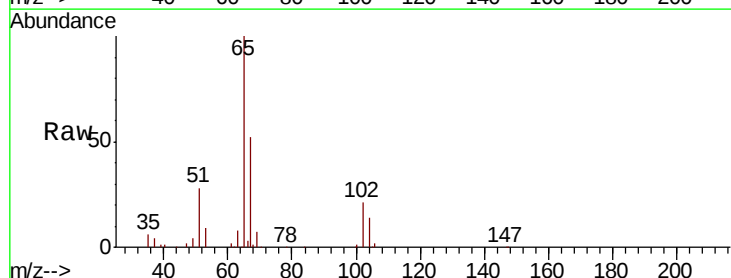

Abundance Ion 64.90 (64.60 to 65.60): VDC

Ion 66.90 (66.60 to 67.60): VDC

8.33

80000


60000


40000

20000

0

Time-->

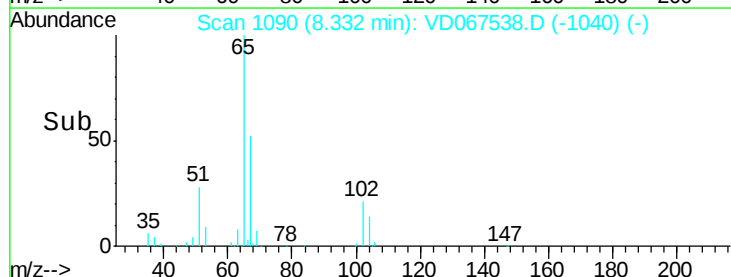

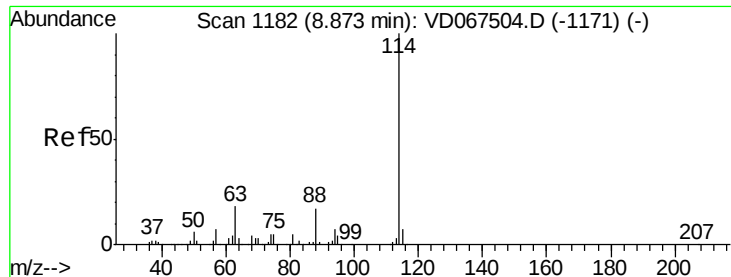

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 8.87 min Scan# 1181

Delta R.T. -0.01 min

Lab File: VD067538.D

Acq: 05 Nov 2020 13:20

Instrument :

MSVOA_D

ClientSampleId :

356


Tot Ion:114 Resp: 502540

Ion Ratio Lower Upper

114 100

63 17.4 0.0 35.0

88 15.2 0.0 33.0

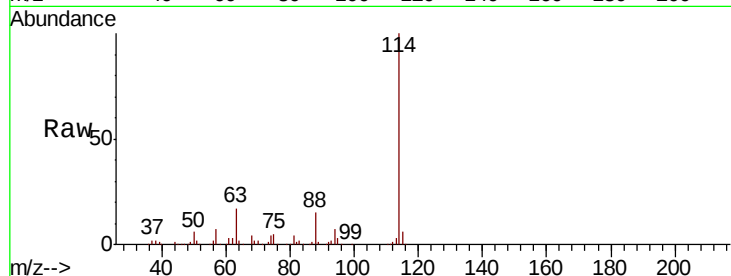

Abundance Ion 113.90 (113.60 to 114.60): V

Ion 63.00 (62.70 to 63.70): V

Ion 87.90 (87.60 to 88.60): V

8.87



300000

200000

100000

0

Time-->

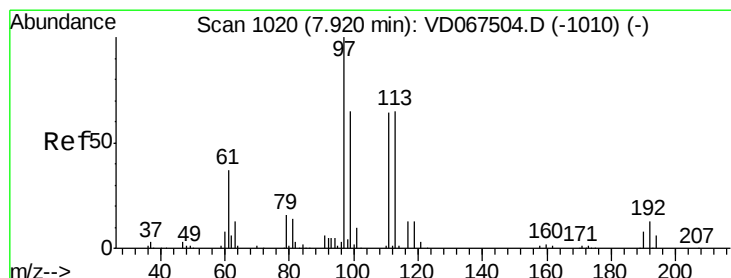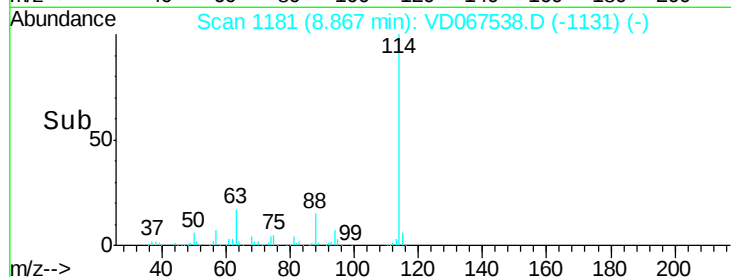

#35

Dibromofluoromethane

Concen: 54.120 ug/l

RT: 7.91 min Scan# 1019

Delta R.T. -0.01 min

Lab File: VD067538.D

Acq: 05 Nov 2020 13:20


Tgt Ion:113 Resp: 163863

Ion Ratio Lower Upper

113 100

111 103.1 80.0 120.0

192 21.1 16.3 24.5

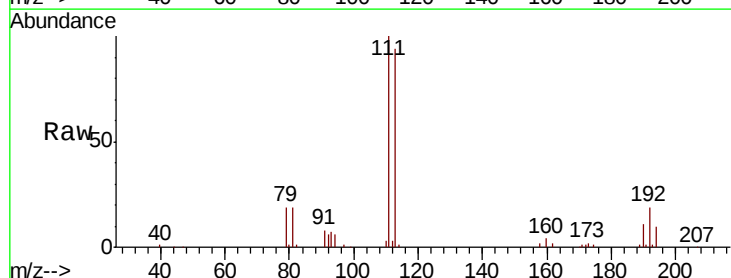

Abundance Ion 112.80 (112.50 to 113.50): V

Ion 110.80 (110.50 to 111.50): V

Ion 191.70 (191.40 to 192.40): V

7.91

80000


60000


40000

20000

0

Time-->

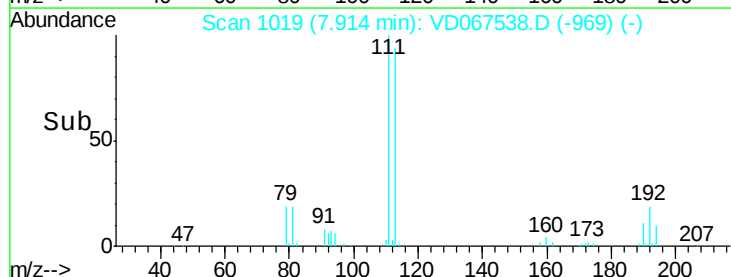

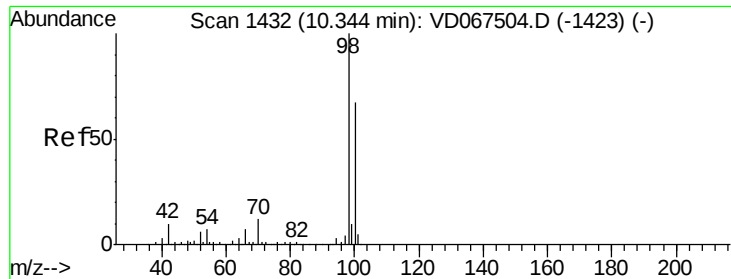

#50

Toluene-d8

Concen: 55.876 ug/l

RT: 10.34 min Scan# 1432

Delta R.T. -0.00 min

Lab File: VD067538.D

Acq: 05 Nov 2020 13:20

Instrument :

MSVOA_D

ClientSampleId :


356

Tot Ion: 98 Resp: 594536

Ion Ratio Lower Upper




98 100

100 66.1 53.0 79.6

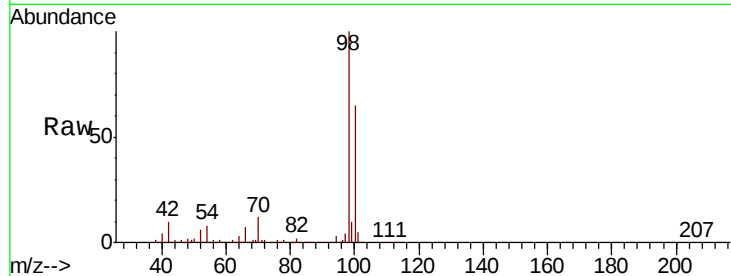

Abundance Ion 98.00 (97.70 to 98.70): VDC

Ion 100.00 (99.70 to 100.70): VDC

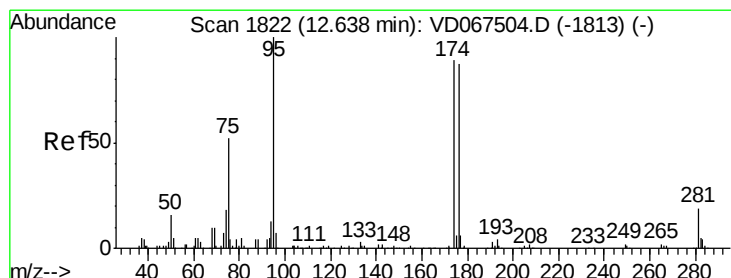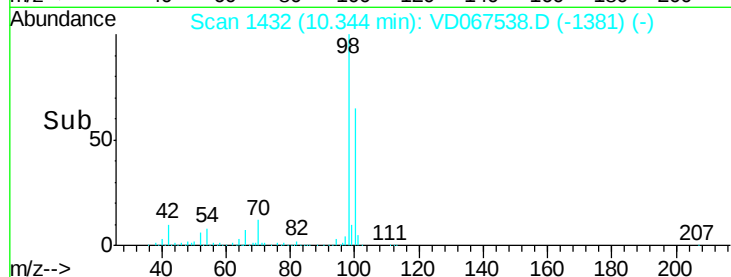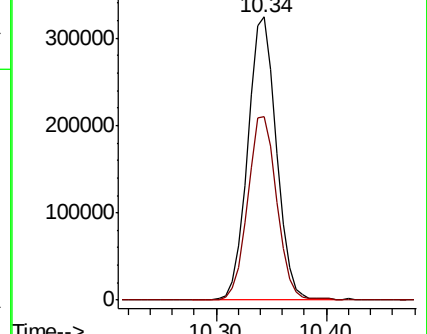

#62

4-Bromofluorobenzene

Concen: 61.748 ug/l

RT: 12.64 min Scan# 1822

Delta R.T. -0.00 min

Lab File: VD067538.D

Acq: 05 Nov 2020 13:20


Tgt Ion: 95 Resp: 226833

Ion Ratio Lower Upper

95 100

174 88.0 0.0 177.8



176 86.7 0.0 172.0

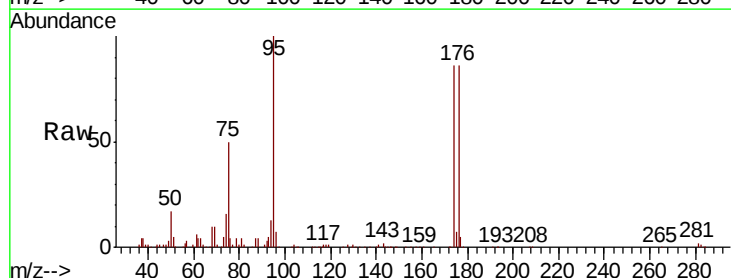


Abundance Ion 94.90 (94.60 to 95.60): VDC

Ion 173.80 (173.50 to 174.50): VDC

Ion 175.80 (175.50 to 176.50): VDC



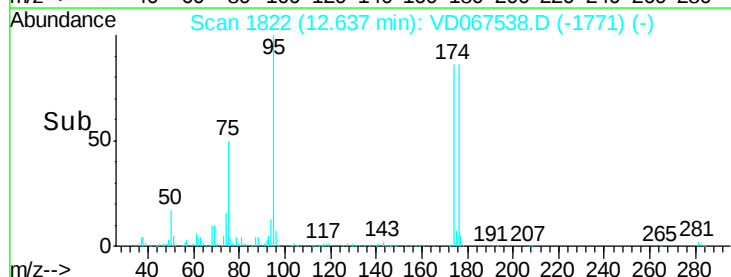
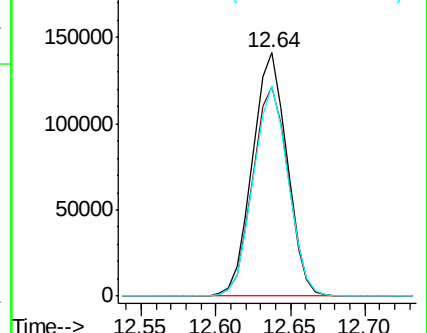


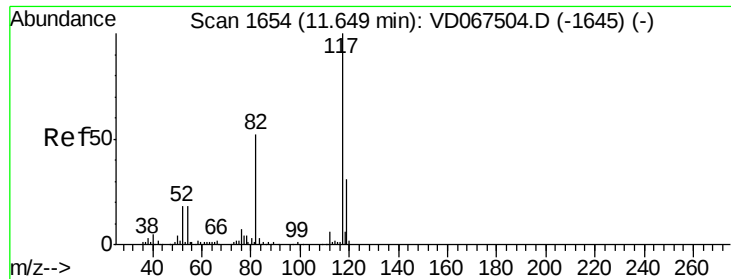

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.65 min Scan# 1654
Delta R.T. -0.00 min
Lab File: VD067538.D
Acq: 05 Nov 2020 13:20

Instrument :
MSVOA_D
ClientSampleId :
356

Tot Ion:117 Resp: 516130
Ion Ratio Lower Upper
117 100
82 50.6 41.6 62.4
119 31.2 25.1 37.7

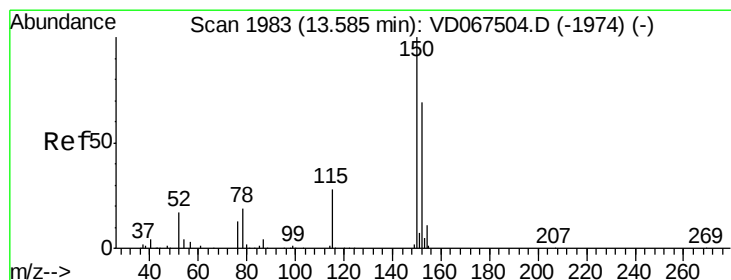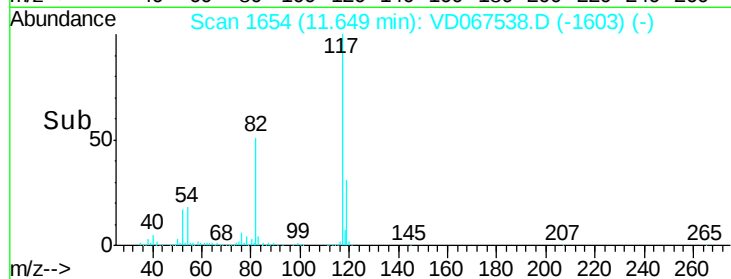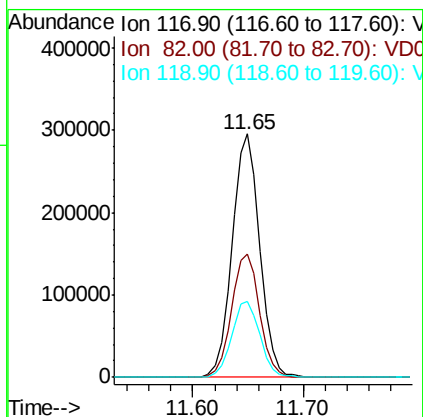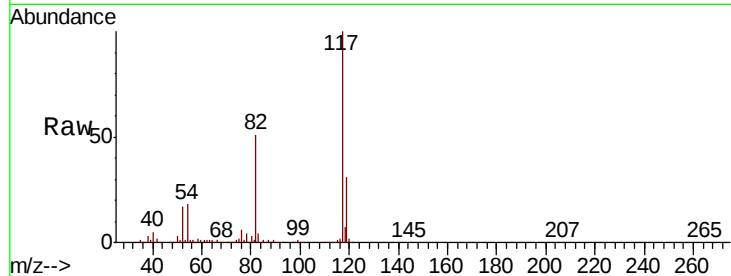

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.58 min Scan# 1982
Delta R.T. -0.01 min
Lab File: VD067538.D
Acq: 05 Nov 2020 13:20

Tgt Ion:152 Resp: 250986
Ion Ratio Lower Upper
152 100
115 59.7 29.3 88.0
150 157.5 0.0 338.2

