

Data Path : Z:\VOASRV\HPCHEM1\MSVOA D\DATA\VD111020\
 Data File : VD067584.D
 Acq On : 10 Nov 2020 16:00
 Operator : VA/SY
 Sample : L4697-06
 Misc : 8.08G/5.00ml/MSVOA D/SOIL
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_D
 ClientSampleId :
 TP-2-D2

Quant Time: Nov 11 00:50:50 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_D\METHOD\82D110320S.M
 Quant Title : SW846 8260
 QLast Update : Wed Nov 04 00:56:28 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	7.98	168	268307	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	8.87	114	447733	50.00	ug/l	0.00
63) Chlorobenzene-d5	11.65	117	425637	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.58	152	234638	50.00	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.33	65	130416	55.59	ug/l	0.00
Spiked Amount	50.000		Recovery	=	111.18%	
35) Dibromofluoromethane	7.92	113	144405	53.53	ug/l	0.00
Spiked Amount	50.000		Recovery	=	107.06%	
50) Toluene-d8	10.34	98	517113	54.55	ug/l	0.00
Spiked Amount	50.000		Recovery	=	109.10%	
62) 4-Bromofluorobenzene	12.64	95	193520	59.13	ug/l	0.00
Spiked Amount	50.000		Recovery	=	118.26%	


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA D\DATA\VD111020\
Data File : VD067584.D
Acq On : 10 Nov 2020 16:00
Operator : VA/SY
Sample : L4697-06
Misc : 8.08G/5.00ml/MSVOA D/SOIL
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
TP-2-D2

Quant Time: Nov 11 00:50:50 2020
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_D\METHOD\82D110320S.M
Quant Title : SW846 8260
QLast Update : Wed Nov 04 00:56:28 2020
Response via : Initial Calibration

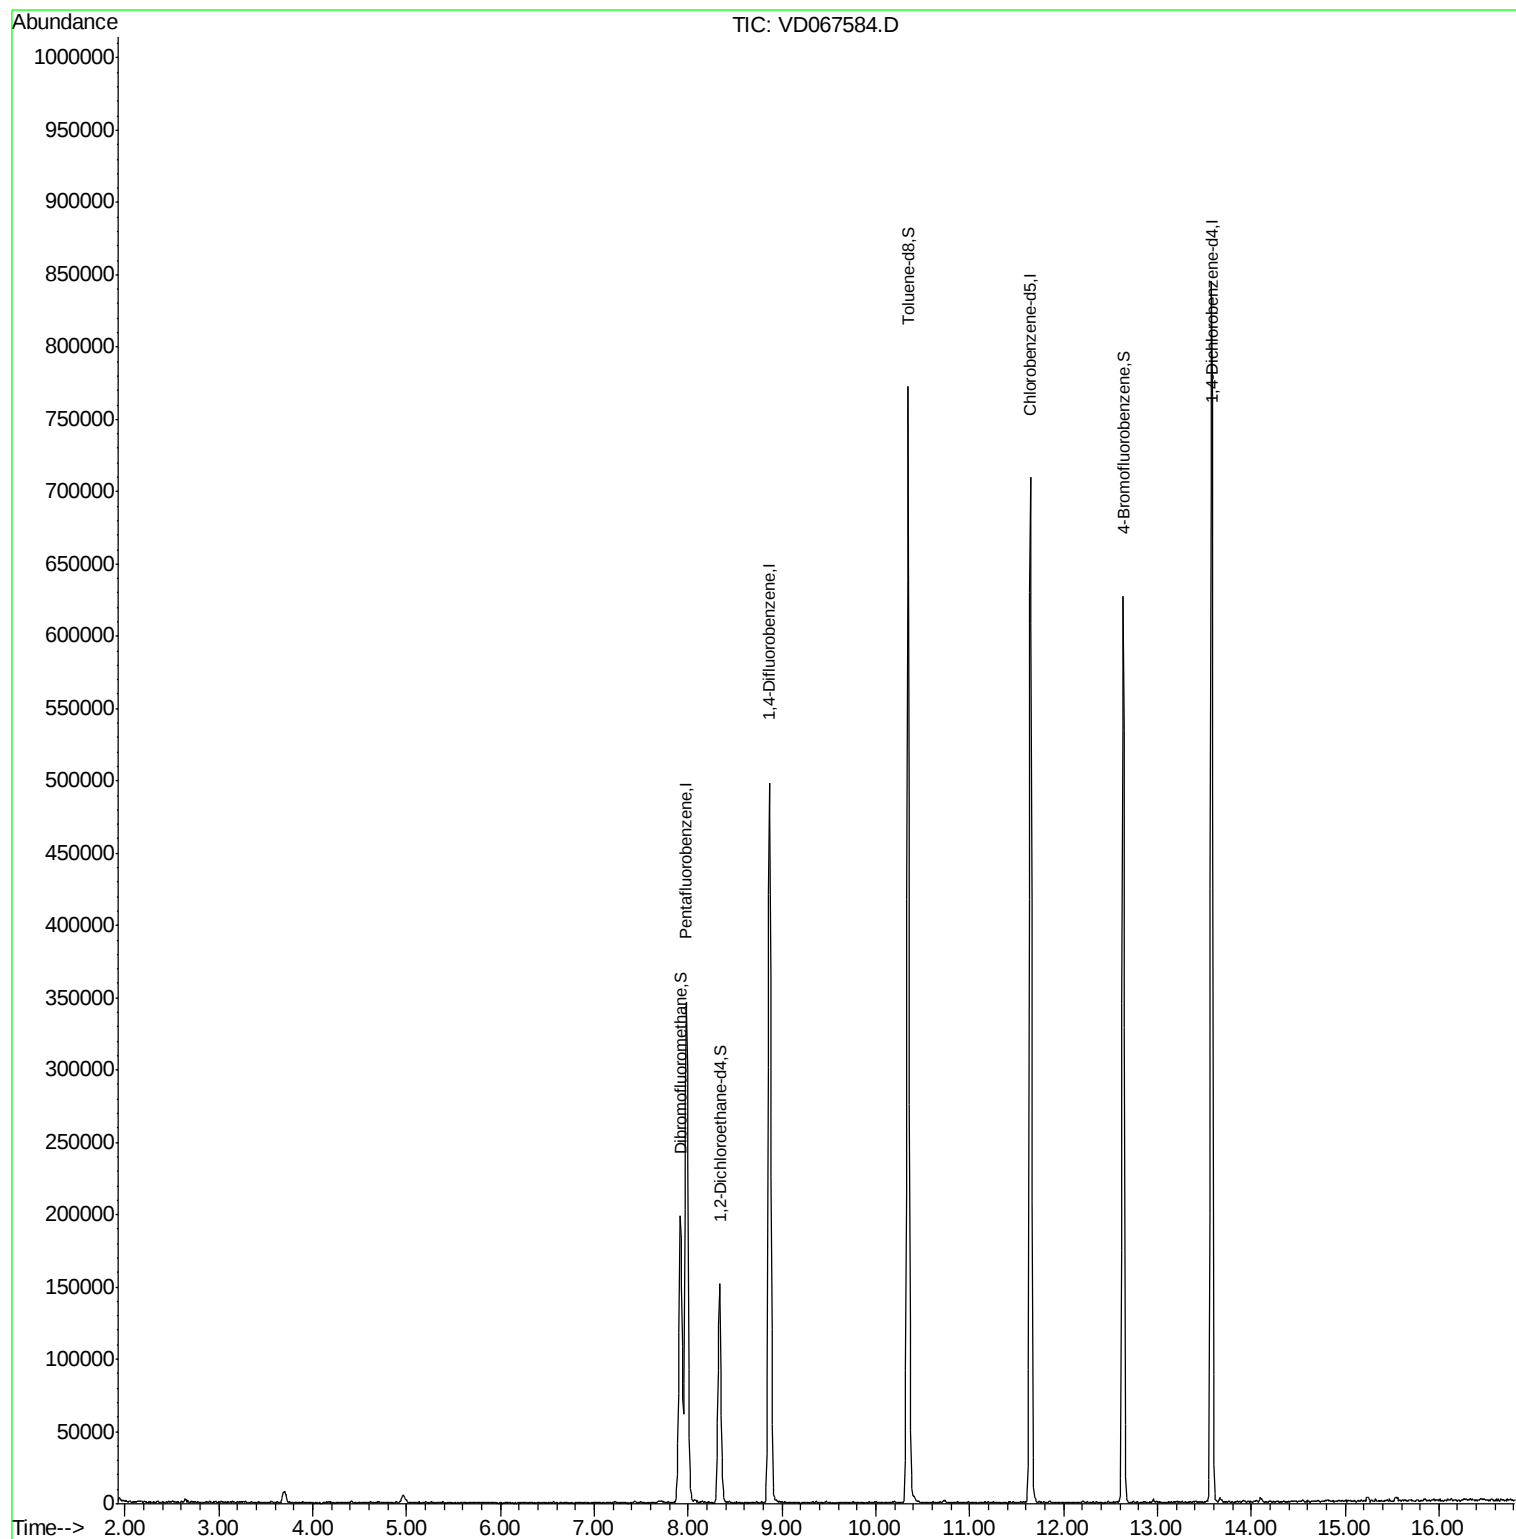

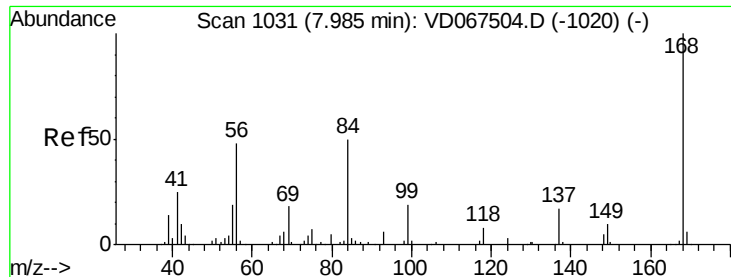

#1

Pentafluorobenzene

Concen: 50.000 ug/l

RT: 7.98 min Scan# 1030

Delta R.T. -0.01 min

Lab File: VD067584.D

Acq: 10 Nov 2020 16:00

Instrument :

MSVOA_D

ClientSampleId :


TP-2-D2

Tot Ion:168 Resp: 268307

Ion Ratio Lower Upper

168 100

99 55.4 45.0 67.6

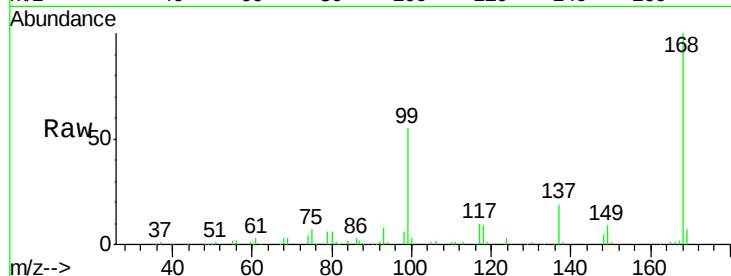

Abundance Ion 167.90 (167.60 to 168.60): V

Ion 98.90 (98.60 to 99.60): VDC



7.98

100000

50000

0

Time-->

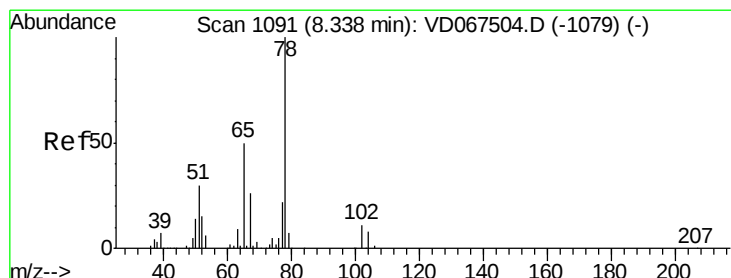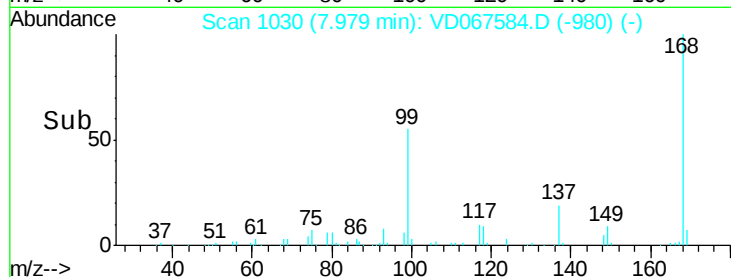

#33

1,2-Dichloroethane-d4

Concen: 55.590 ug/l

RT: 8.33 min Scan# 1090

Delta R.T. -0.01 min

Lab File: VD067584.D


Acq: 10 Nov 2020 16:00

Tgt Ion: 65 Resp: 130416

Ion Ratio Lower Upper

65 100

67 48.2 0.0 99.4

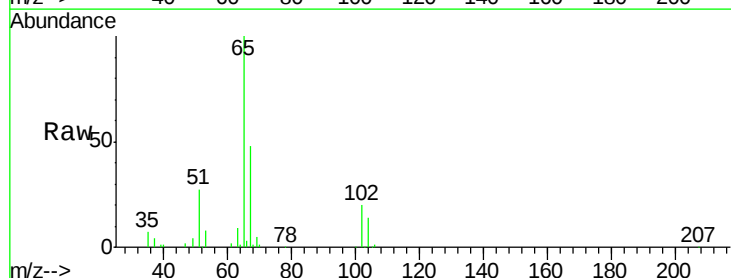

Abundance Ion 64.90 (64.60 to 65.60): VDC

Ion 66.90 (66.60 to 67.60): VDC

8.33

60000

50000

40000


30000


20000

10000

0

Time-->

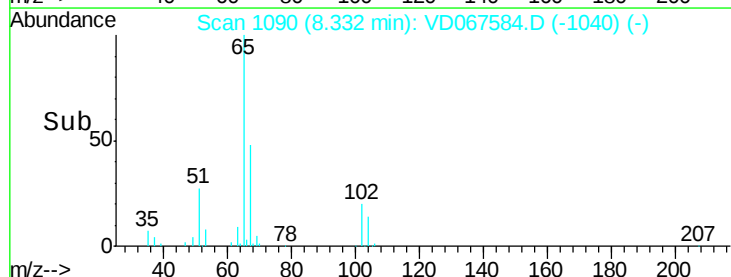

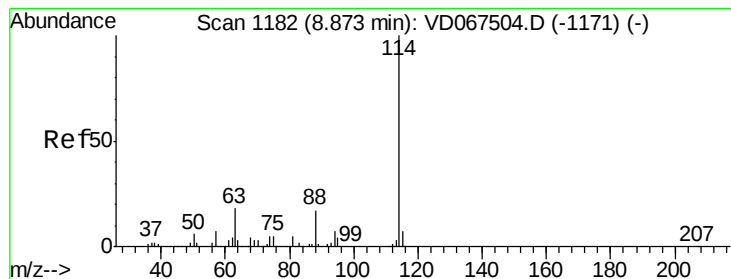

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 8.87 min Scan# 1181

Delta R.T. -0.01 min

Lab File: VD067584.D

Acq: 10 Nov 2020 16:00

Instrument :

MSVOA_D

ClientSampleId :

TP-2-D2


Tot Ion:114 Resp: 447733

Ion Ratio Lower Upper

114 100

63 17.1 0.0 35.0




88 16.3 0.0 33.0

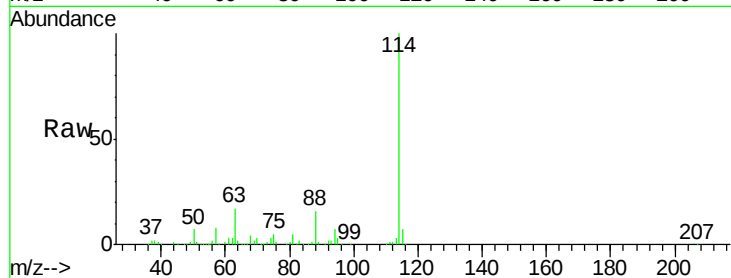

Abundance Ion 113.90 (113.60 to 114.60): V

Ion 63.00 (62.70 to 63.70): V

Ion 87.90 (87.60 to 88.60): V

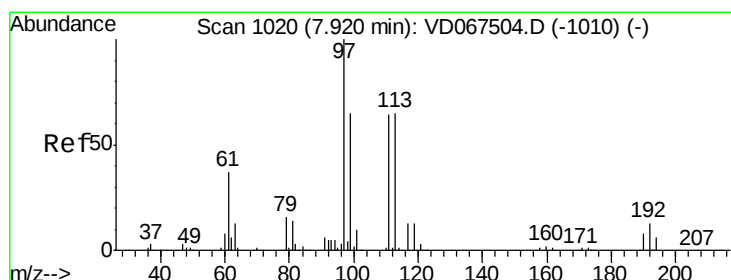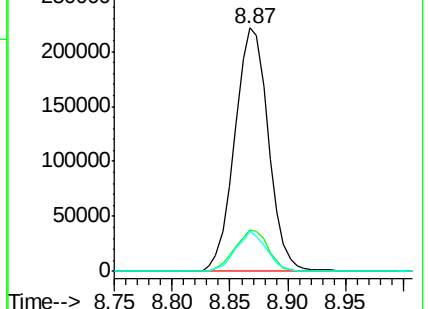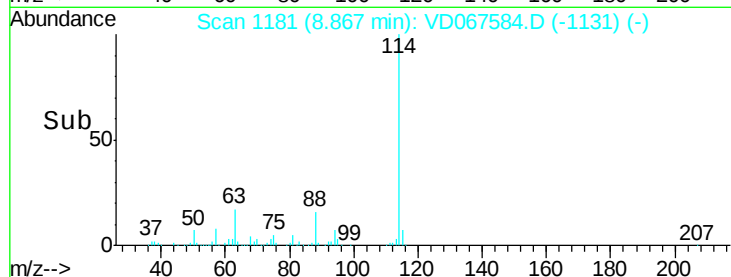

#35

Dibromofluoromethane

Concen: 53.531 ug/l

RT: 7.92 min Scan# 1020

Delta R.T. -0.00 min

Lab File: VD067584.D

Acq: 10 Nov 2020 16:00


Tgt Ion:113 Resp: 144405

Ion Ratio Lower Upper

113 100

111 101.8 80.0 120.0



192 21.1 16.3 24.5

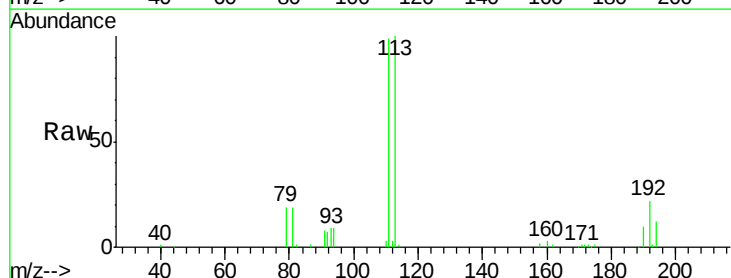


Abundance Ion 112.80 (112.50 to 113.50): V

Ion 110.80 (110.50 to 111.50): V

Ion 191.70 (191.40 to 192.40): V


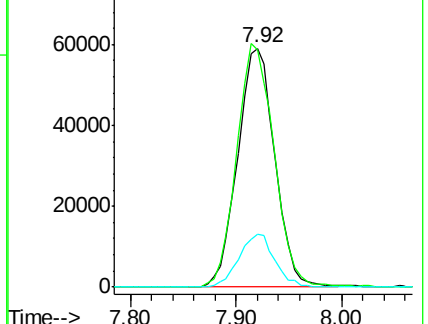
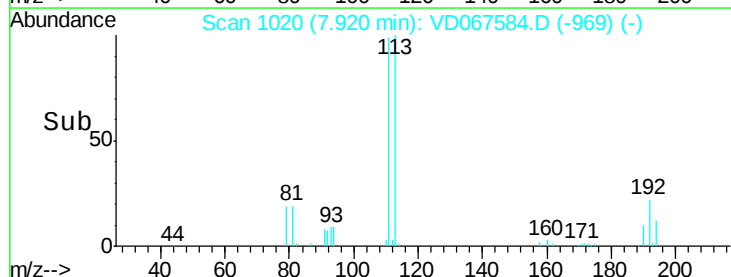


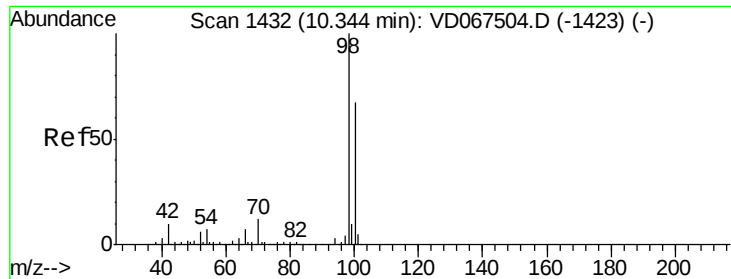

#50
Toluene-d8
Concen: 54.548 ug/l
RT: 10.34 min Scan# 1432
Delta R.T. -0.00 min
Lab File: VD067584.D
Acq: 10 Nov 2020 16:00




Instrument :
MSVOA_D
ClientSampleId :
TP-2-D2


Tot Ion: 98 Resp: 517113
Ion Ratio Lower Upper
98 100
100 66.6 53.0 79.6

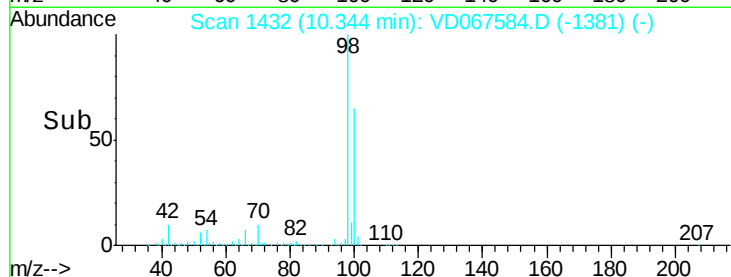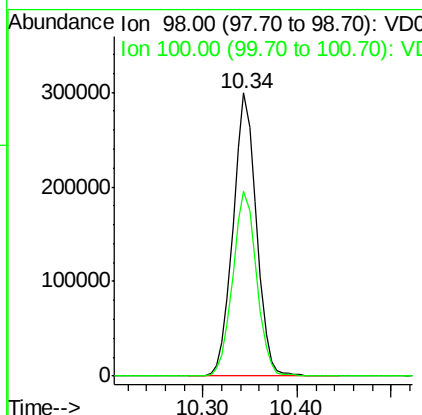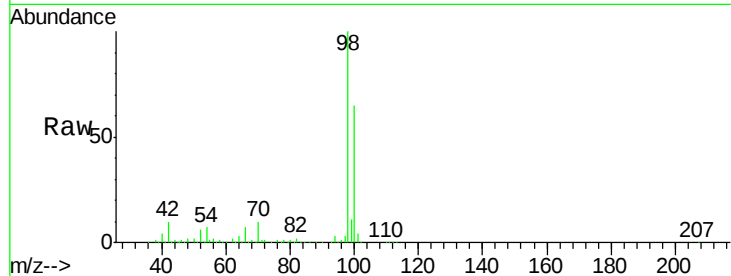

#62
4-Bromofluorobenzene
Concen: 59.128 ug/l
RT: 12.64 min Scan# 1822
Delta R.T. -0.00 min
Lab File: VD067584.D
Acq: 10 Nov 2020 16:00

Tgt Ion: 95 Resp: 193520
Ion Ratio Lower Upper
95 100
174 92.8 0.0 177.8
176 89.1 0.0 172.0


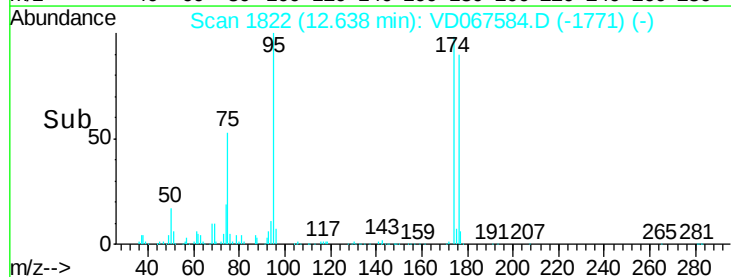
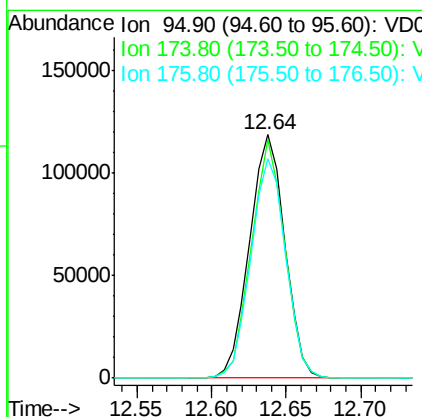
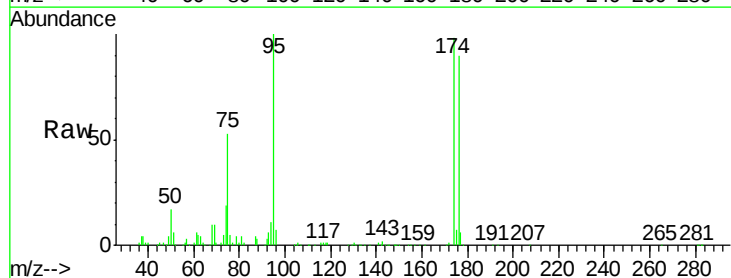


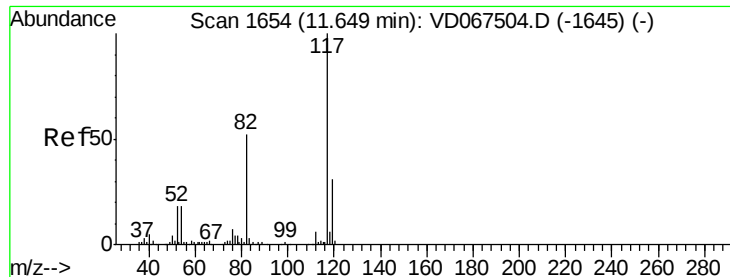

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.65 min Scan# 1654
Delta R.T. -0.00 min
Lab File: VD067584.D
Acq: 10 Nov 2020 16:00

Instrument :
MSVOA_D
ClientSampleId :
TP-2-D2

Tot Ion:117 Resp: 425637
Ion Ratio Lower Upper
117 100
82 52.3 41.6 62.4
119 33.2 25.1 37.7

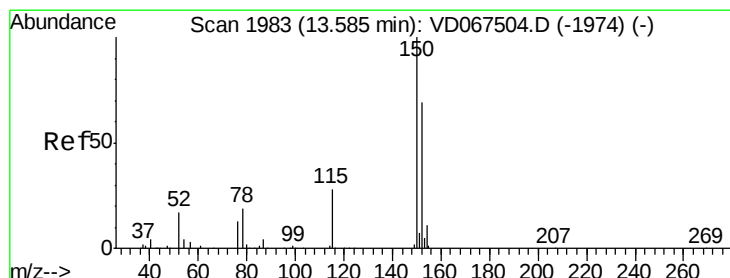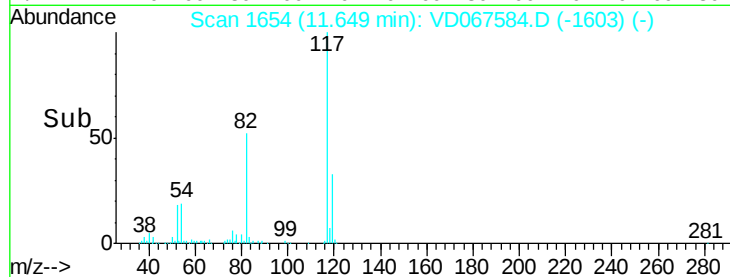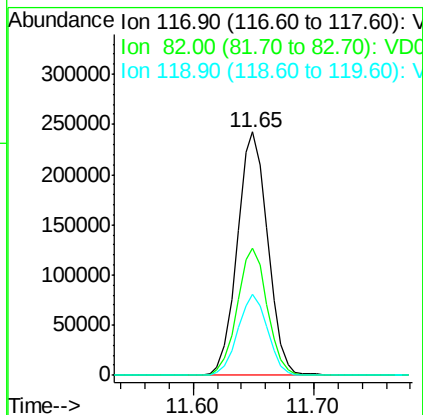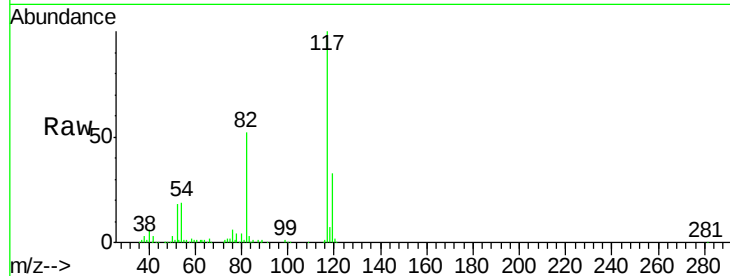

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.58 min Scan# 1982
Delta R.T. -0.01 min
Lab File: VD067584.D
Acq: 10 Nov 2020 16:00

Tgt Ion:152 Resp: 234638
Ion Ratio Lower Upper
152 100
115 59.7 29.3 88.0
150 157.7 0.0 338.2

