

Data Path : Z:\VOASRV\HPCHEM1\MSVOA D\DATA\VD111120\
 Data File : VD067607.D
 Acq On : 11 Nov 2020 17:25
 Operator : VA/SY
 Sample : L4706-02
 Misc : 6.37G/5.00ml/MSVOA D/SOIL
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_D
 ClientSampleId :
 16874

Quant Time: Nov 12 00:10:48 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_D\METHOD\82D110320S.M
 Quant Title : SW846 8260
 QLast Update : Wed Nov 04 00:56:28 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	7.98	168	47105	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	8.87	114	71772	50.00	ug/l	0.00
63) Chlorobenzene-d5	11.65	117	79211	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.58	152	39227	50.00	ug/l	0.00

System Monitoring Compounds

33) 1,2-Dichloroethane-d4	8.34	65	31071	75.44	ug/l	0.00
Spiked Amount	50.000		Recovery	=	150.88%	
35) Dibromofluoromethane	7.92	113	27039	62.53	ug/l	0.00
Spiked Amount	50.000		Recovery	=	125.06%	
50) Toluene-d8	10.34	98	86892	57.18	ug/l	0.00
Spiked Amount	50.000		Recovery	=	114.36%	
62) 4-Bromofluorobenzene	12.64	95	37287	71.07	ug/l	0.00
Spiked Amount	50.000		Recovery	=	142.14%	

Target Compounds


						Qvalue
3) Chloromethane	2.32	50	461	1.572	ug/l #	41
11) Tert butyl alcohol	5.22	59	2507	131.683	ug/l #	90
15) Acrylonitrile	5.68	53	104	1.649	ug/l #	18
16) Acetone	4.16	43	43757	709.928	ug/l	99
18) Methyl Acetate	4.71	43	448	3.517	ug/l #	41
20) Methylene Chloride	4.97	84	591	1.357	ug/l #	14
25) 2-Butanone	7.22	43	13832	210.023	ug/l	94
29) Tetrahydrofuran	7.56	42	258	6.540	ug/l #	63
36) 1,1-Dichloropropene	7.98	75	3599	5.858	ug/l #	45
37) Ethyl Acetate	7.22	43	13832	86.722	ug/l #	63
38) Carbon Tetrachloride	7.97	117	4930	6.176	ug/l #	12
40) Benzene	8.36	78	5315	3.194	ug/l	91
41) Methacrylonitrile	7.54	41	98	1.028	ug/l #	13
48) Methyl methacrylate	9.44	41	1572	9.652	ug/l #	31
51) 4-Methyl-2-Pentanone	10.23	43	18542	122.909	ug/l	97
52) Toluene	10.41	92	6643	5.960	ug/l	92
56) Ethyl methacrylate	10.76	69	402	1.286	ug/l #	1
59) 2-Hexanone	10.98	43	5973	56.626	ug/l	81
68) m/p-Xylenes	11.86	106	6427	6.327	ug/l	98
69) o-Xylene	12.18	106	11274	12.431	ug/l	88
71) Bromoform	12.64	173	413	1.347	ug/l #	29
74) N-amyl acetate	12.26	43	34447	103.262	ug/l #	42
75) 1,1,2,2-Tetrachloroethane	12.76	83	501	1.449	ug/l #	26
76) 1,2,3-Trichloropropane	12.64	75	19277	81.461	ug/l #	100
81) trans-1,4-Dichloro-2-buten	12.47	75	655	5.620	ug/l #	24
84) 1,2,4-Trimethylbenzene	13.27	105	2612	1.212	ug/l	86
95) Naphthalene	15.41	128	2564	2.381	ug/l #	77


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA D\DATA\VD111120\
Data File : VD067607.D
Acq On : 11 Nov 2020 17:25
Operator : VA/SY
Sample : L4706-02
Misc : 6.37G/5.00ml/MSVOA D/SOIL
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
16874

Quant Time: Nov 12 00:10:48 2020
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_D\METHOD\82D110320S.M
Quant Title : SW846 8260
QLast Update : Wed Nov 04 00:56:28 2020
Response via : Initial Calibration

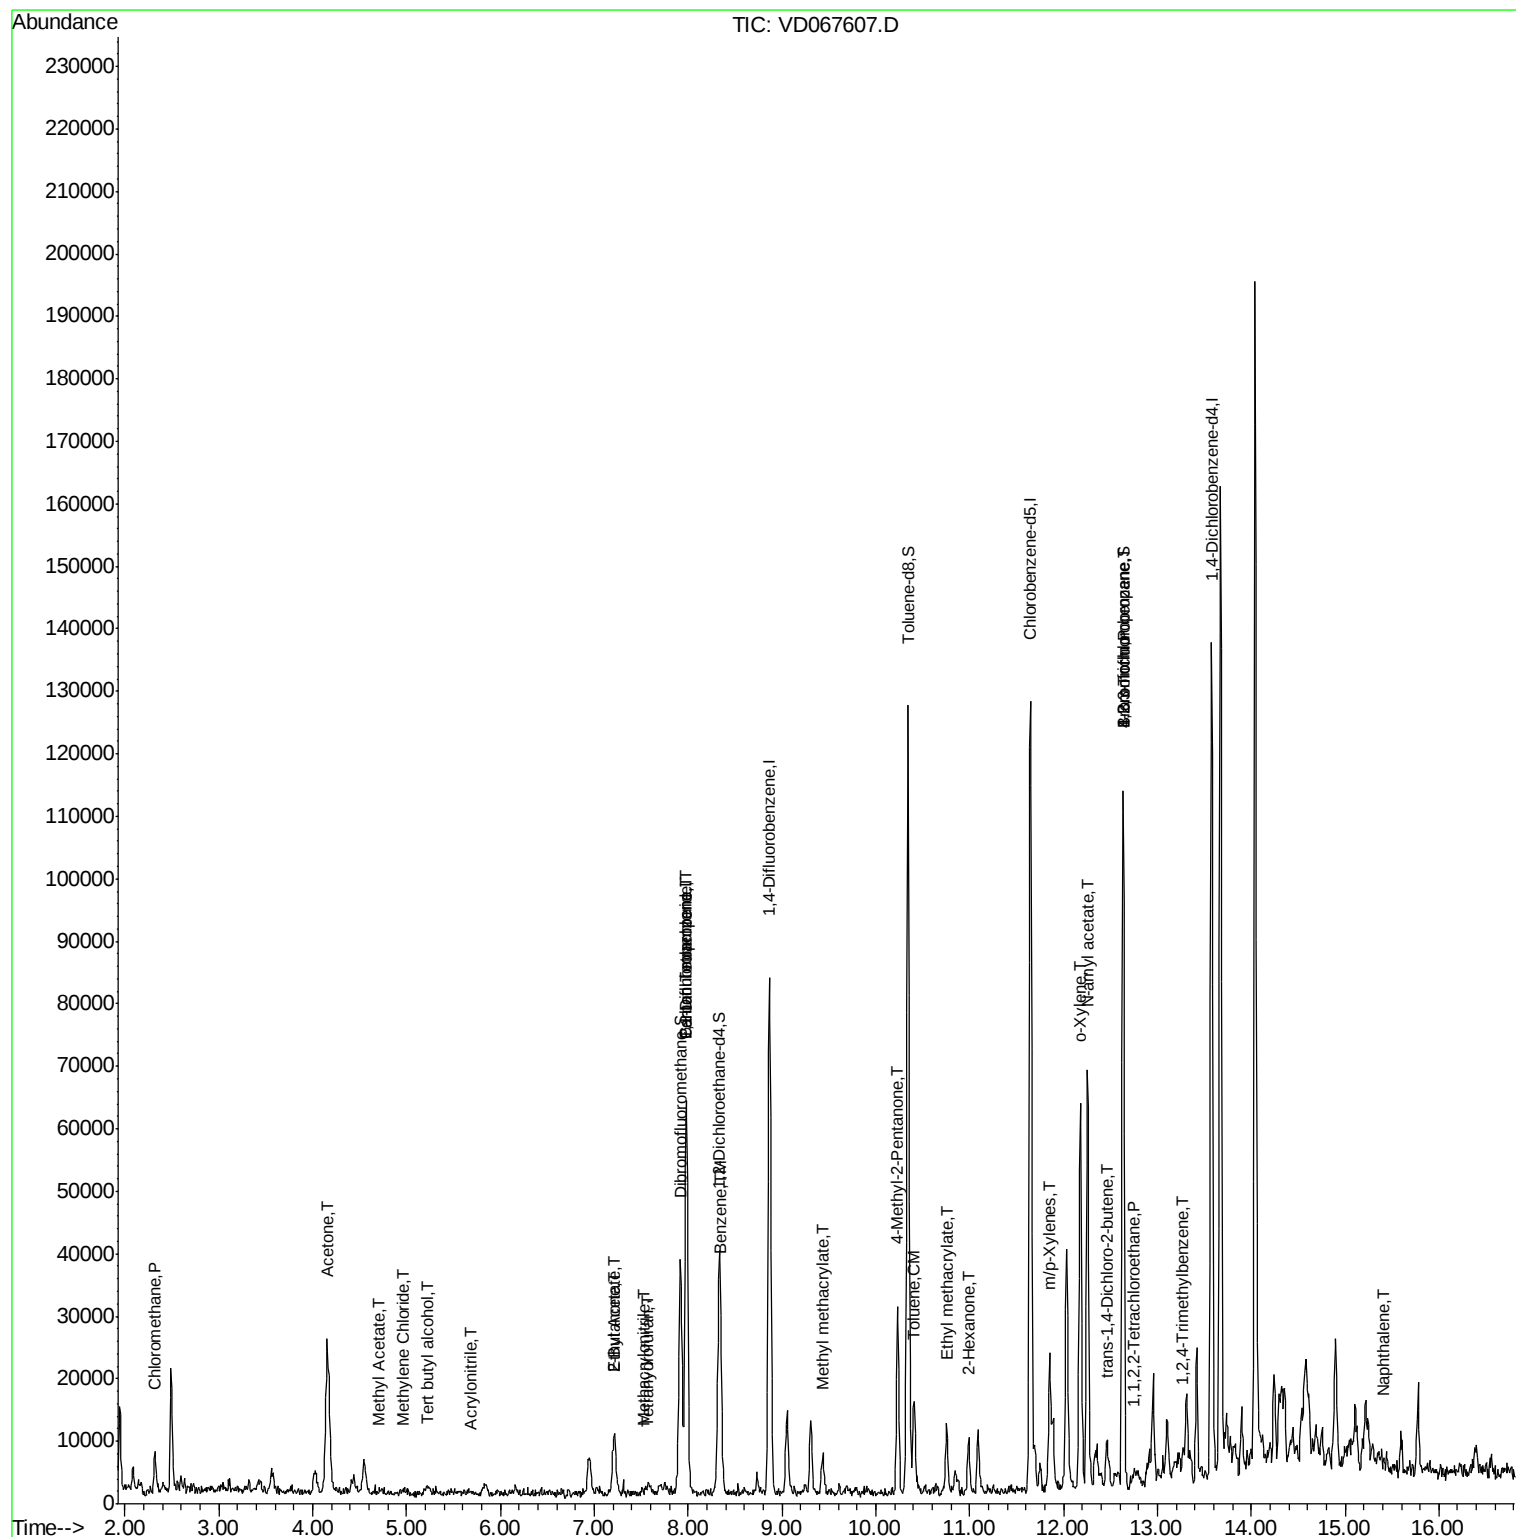



#1

Pentafluorobenzene

Concen: 50.000 ug/l

RT: 7.98 min Scan# 1031

Delta R.T. -0.00 min

Lab File: VD067607.D

Acq: 11 Nov 2020 17:25

Instrument :

MSVOA_D

ClientSampleId :


16874

Tot Ion:168 Resp: 47105

Ion Ratio Lower Upper

168 100

99 52.3 45.0 67.6

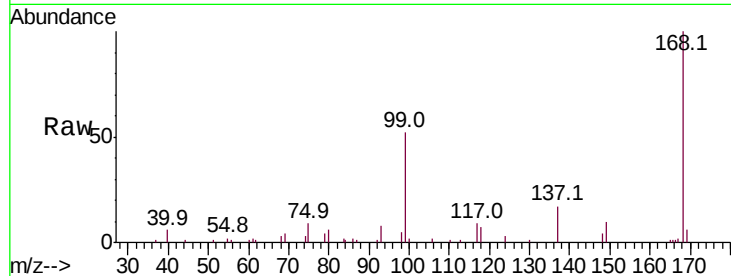

Abundance Ion 167.90 (167.60 to 168.60): V

Ion 98.90 (98.60 to 99.60): VDC

7.98

25000

20000

15000



10000

5000

0

Time-->

7.90 7.95 8.00 8.05 8.10



#3

Chloromethane

Concen: 1.572 ug/l

RT: 2.32 min Scan# 68

Delta R.T. 0.11 min

Lab File: VD067607.D


Acq: 11 Nov 2020 17:25

Tgt Ion: 50 Resp: 461

Ion Ratio Lower Upper

50 100

52 0.0 27.3 40.9#



Abundance Ion 49.90 (49.60 to 50.60): VDC

Ion 51.90 (51.60 to 52.60): VDC

2.32

600

500

400

300


200


100

0

Time-->

2.28 2.30 2.32 2.34






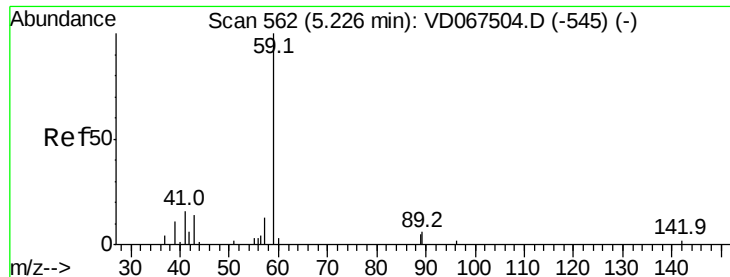


#11

Tert butyl alcohol
 Concen: 131.683 ug/l
 RT: 5.22 min Scan# 561
 Delta R.T. -0.01 min
 Lab File: VD067607.D
 Acq: 11 Nov 2020 17:25

Instrument :
 MSVOA_D
 ClientSampleId :
 16874




Tot Ion: 59 Resp: 2507
 Ion Ratio Lower Upper
 59 100
 57 4.0 5.9 8.9#

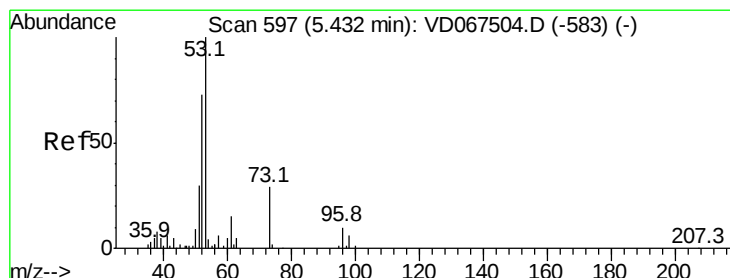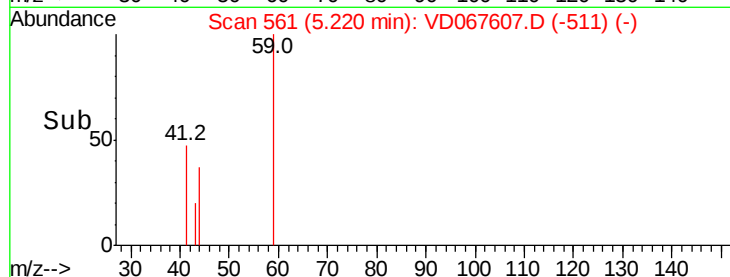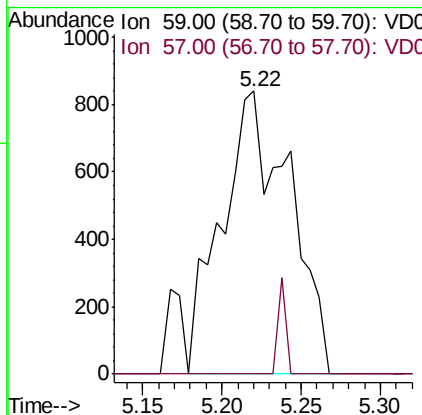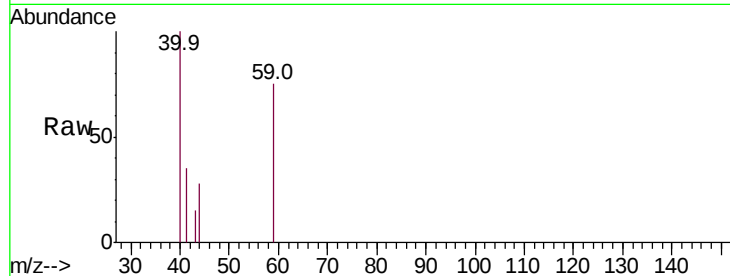


#15

Acrylonitrile
 Concen: 1.649 ug/l
 RT: 5.68 min Scan# 639
 Delta R.T. 0.25 min
 Lab File: VD067607.D
 Acq: 11 Nov 2020 17:25

Tgt Ion: 53 Resp: 104
 Ion Ratio Lower Upper
 53 100
 52 0.0 64.8 97.2#
 51 0.0 29.5 44.3#

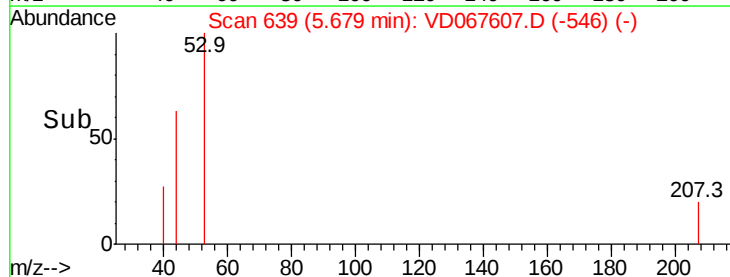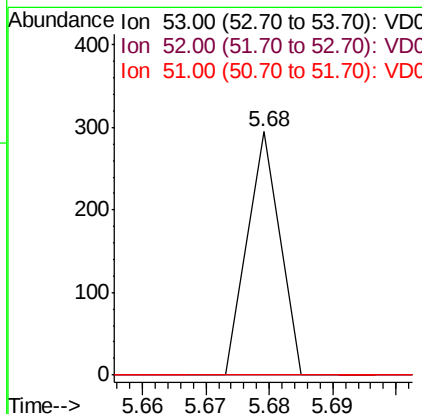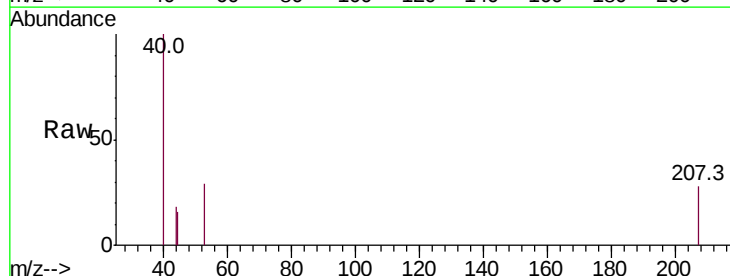



#16

Acetone

Concen: 709.928 ug/l

RT: 4.16 min Scan# 381

Delta R.T. 0.01 min

Lab File: VD067607.D

Acq: 11 Nov 2020 17:25

Instrument :

MSVOA_D

ClientSampleId :





16874

Tot Ion: 43 Resp: 43757

Ion Ratio Lower Upper

43 100

58 31.2 25.2 37.8

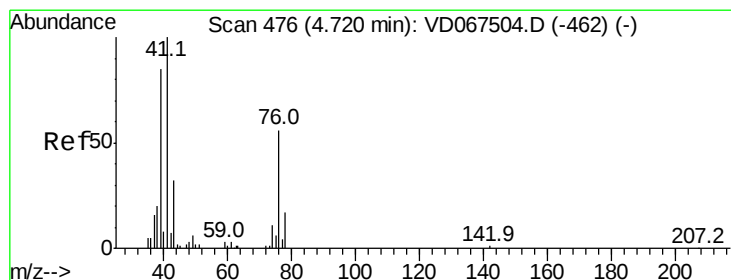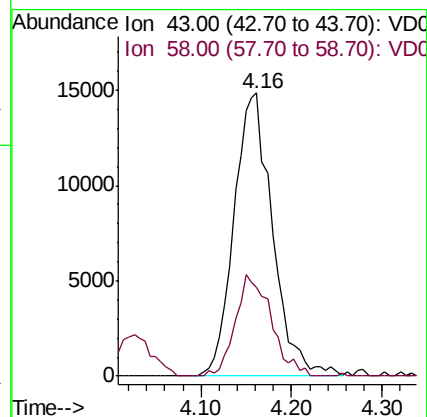

#18

Methyl Acetate

Concen: 3.517 ug/l

RT: 4.71 min Scan# 474

Delta R.T. -0.01 min

Lab File: VD067607.D




Acq: 11 Nov 2020 17:25


Tgt Ion: 43 Resp: 448

Ion Ratio Lower Upper

43 100

74 0.0 27.2 40.8#



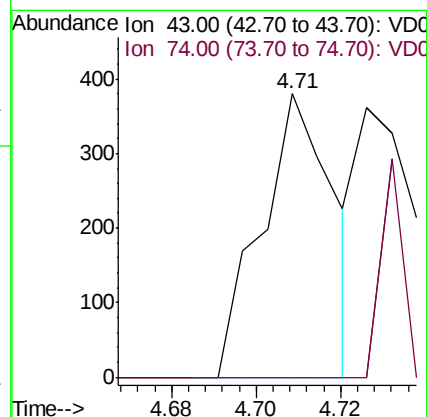
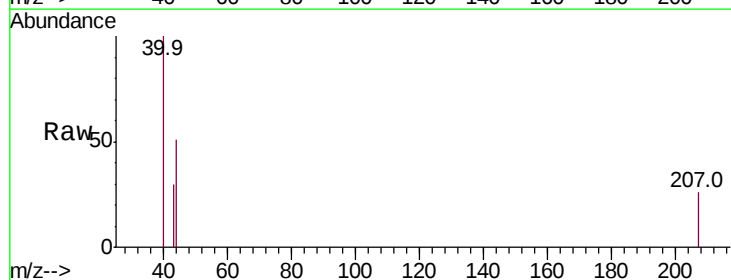




#20
Methvlene Chloride
Concen: 1.357 ug/l
RT: 4.97 min Scan# 518
Delta R.T. -0.00 min
Lab File: VD067607.D
Acq: 11 Nov 2020 17:25




Instrument :
MSVOA_D
ClientSampleId :
16874


Tot Ion: 84 Resp: 591
Ion Ratio Lower Upper
84 100
49 0.0 77.0 115.4#
51 0.0 25.4 38.2#
86 0.0 49.4 74.0#

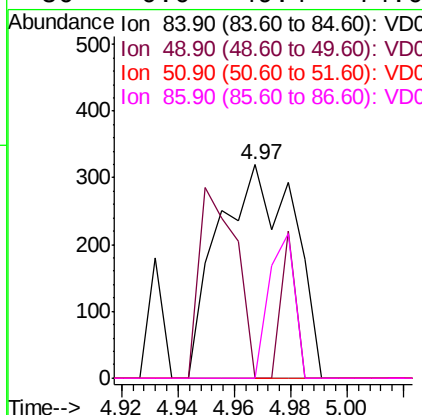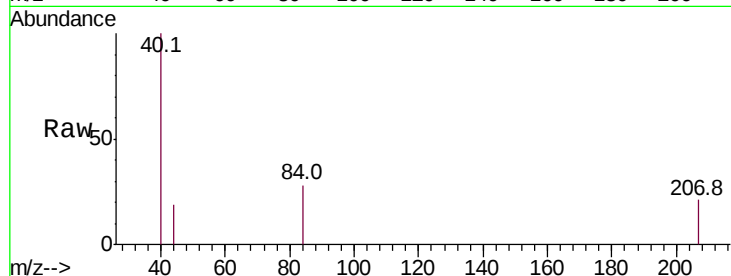

#25
2-Butanone
Concen: 210.023 ug/l
RT: 7.22 min Scan# 901
Delta R.T. 0.01 min
Lab File: VD067607.D
Acq: 11 Nov 2020 17:25

Tgt Ion: 43 Resp: 13832
Ion Ratio Lower Upper
43 100
72 36.5 26.4 39.6

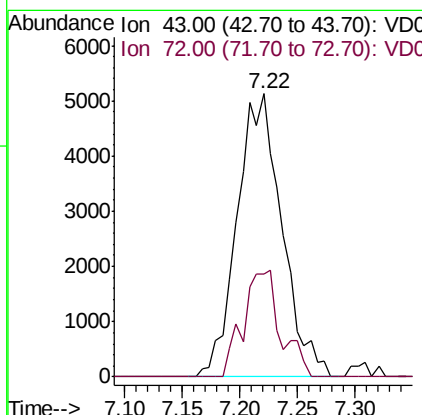



#29

Tetrahydrofuran

Concen: 6.540 ug/l

RT: 7.56 min Scan# 959

Delta R.T. -0.01 min

Lab File: VD067607.D

Acq: 11 Nov 2020 17:25

Instrument :

MSVOA_D

ClientSampled :

16874





Tot Ion: 42 Resp: 258

Ion Ratio Lower Upper

42 100

72 22.1 46.3 69.5#

71 36.8 44.0 66.0#

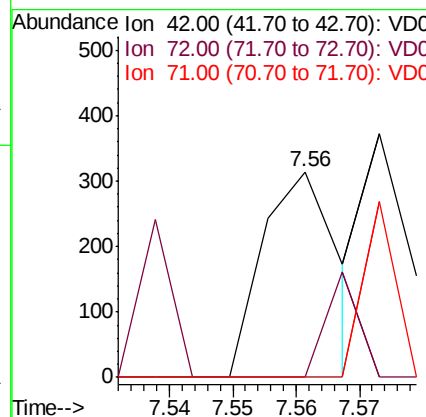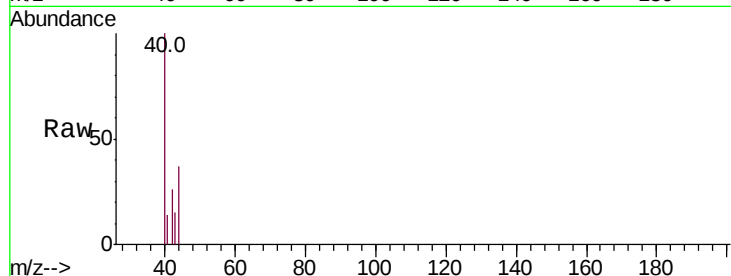

#33

1,2-Dichloroethane-d4

Concen: 75.437 ug/l

RT: 8.34 min Scan# 1091

Delta R.T. -0.00 min

Lab File: VD067607.D




Acq: 11 Nov 2020 17:25


Tgt Ion: 65 Resp: 31071

Ion Ratio Lower Upper

65 100

67 47.9 0.0 99.4

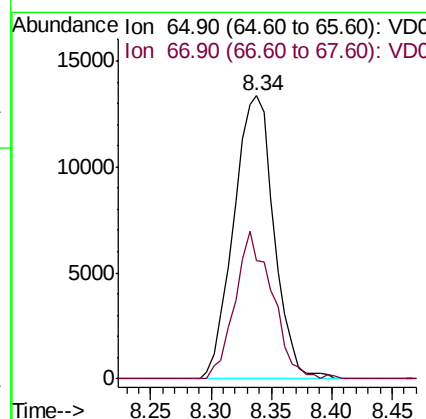



#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 8.87 min Scan# 1181

Delta R.T. -0.01 min

Lab File: VD067607.D

Acq: 11 Nov 2020 17:25

Instrument :

MSVOA_D

ClientSampleId :

16874


Tot Ion:114 Resp: 71772

Ion Ratio Lower Upper

114 100

63 20.0 0.0 35.0




88 15.2 0.0 33.0



Abundance Ion 113.90 (113.60 to 114.60): V

Ion 63.00 (62.70 to 63.70): V

Ion 87.90 (87.60 to 88.60): V

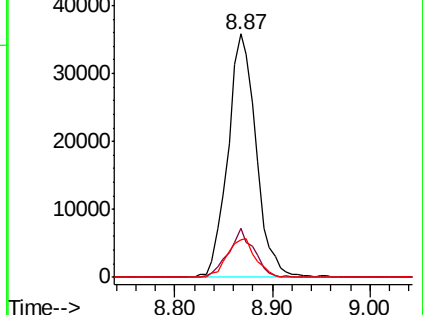

#35

Dibromofluoromethane

Concen: 62.529 ug/l

RT: 7.92 min Scan# 1020

Delta R.T. -0.00 min

Lab File: VD067607.D

Acq: 11 Nov 2020 17:25


Tgt Ion:113 Resp: 27039

Ion Ratio Lower Upper

113 100

111 102.2 80.0 120.0



192 22.2 16.3 24.5




Abundance Ion 112.80 (112.50 to 113.50): V

Ion 110.80 (110.50 to 111.50): V

Ion 191.70 (191.40 to 192.40): V



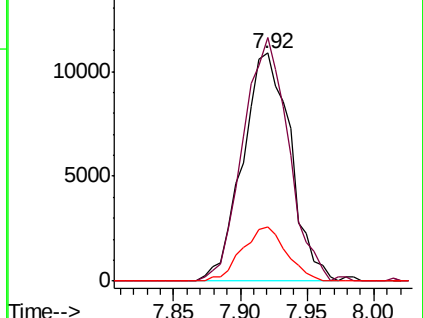





#36
 1,1-Dichloropropene
 Concen: 5.858 ug/l
 RT: 7.98 min Scan# 1031
 Delta R.T. -0.14 min
 Lab File: VD067607.D
 Acq: 11 Nov 2020 17:25




Instrument :
 MSVOA_D
 ClientSampleId :
 16874


Tot Ion: 75 Resp: 3599
 Ion Ratio Lower Upper
 75 100
 110 7.1 19.9 59.7#
 77 0.0 24.8 37.2#

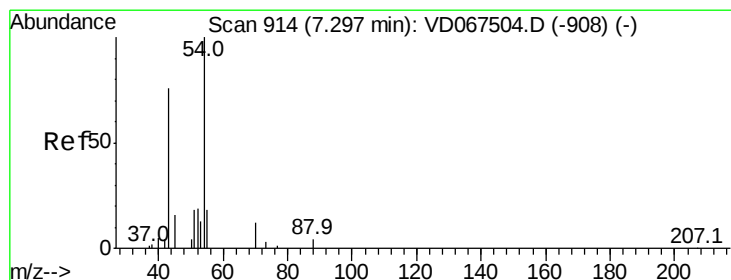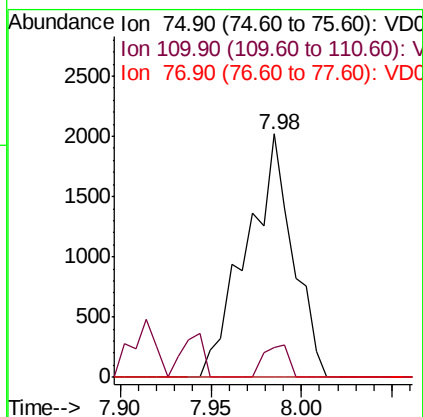

#37
 Ethyl Acetate
 Concen: 86.722 ug/l
 RT: 7.22 min Scan# 901
 Delta R.T. -0.08 min
 Lab File: VD067607.D
 Acq: 11 Nov 2020 17:25

Tgt Ion: 43 Resp: 13832
 Ion Ratio Lower Upper
 43 100
 61 0.0 12.8 19.2#
 70 0.0 11.7 17.5#

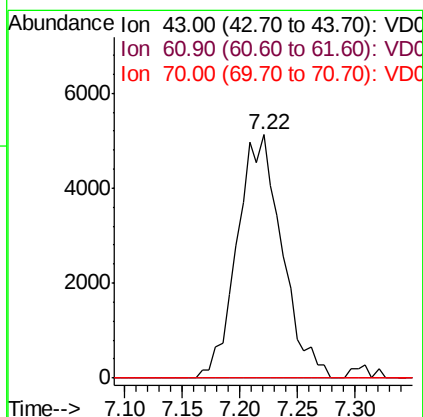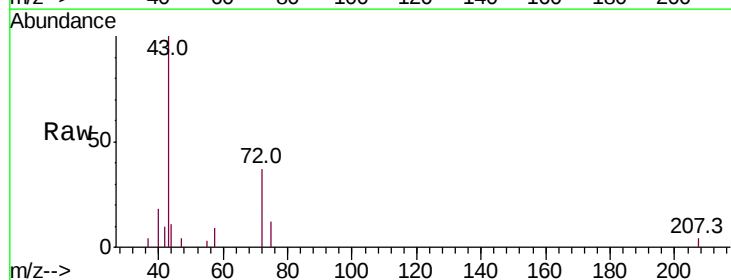



#38

Carbon Tetrachloride

Concen: 6.176 ug/l

RT: 7.97 min Scan# 1029

Delta R.T. -0.13 min

Lab File: VD067607.D

Acq: 11 Nov 2020 17:25

Instrument :

MSVOA_D

ClientSampleId :

16874


Tot Ion:117 Resp: 4930

Ion Ratio Lower Upper

117 100

119 0.0 76.9 115.3#




121 0.0 24.5 36.7#



Abundance Ion 116.80 (116.50 to 117.50): V

Ion 118.80 (118.50 to 119.50): V

Ion 120.80 (120.50 to 121.50): V

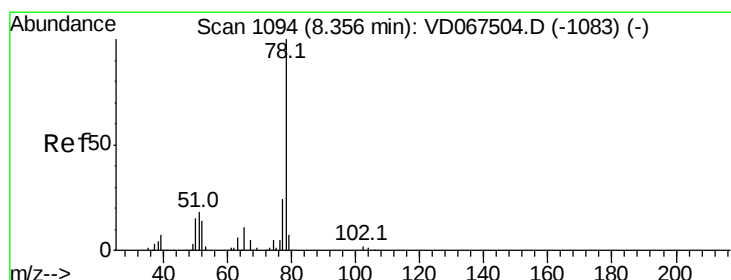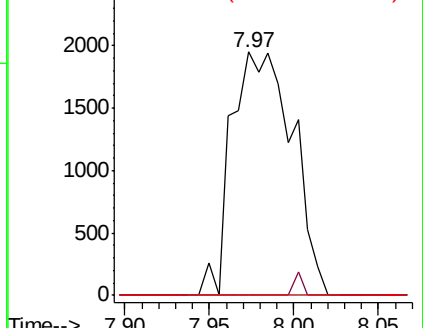

#40

Benzene

Concen: 3.194 ug/l

RT: 8.36 min Scan# 1094

Delta R.T. -0.00 min

Lab File: VD067607.D


Acq: 11 Nov 2020 17:25

Tgt Ion: 78 Resp: 5315

Ion Ratio Lower Upper



78 100


77 19.2 19.1 28.7



Abundance Ion 78.00 (77.70 to 78.70): V

Ion 77.00 (76.70 to 77.70): V

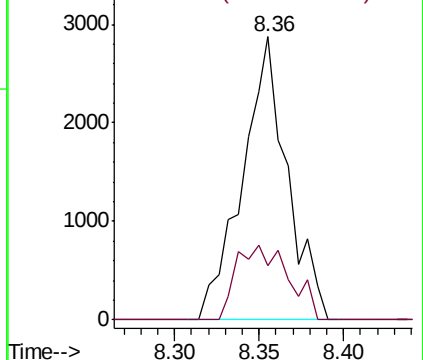







#41
Methacrylonitrile
Concen: 1.028 ug/l
RT: 7.54 min Scan# 955
Delta R.T. 0.01 min
Lab File: VD067607.D
Acq: 11 Nov 2020 17:25

Instrument :
MSVOA_D
ClientSampleId :
16874

Tot Ion: 41 Resp: 98
Ion Ratio Lower Upper
41 100
39 0.0 51.3 76.9#
67 0.0 78.9 118.3#
52 0.0 31.4 47.2#

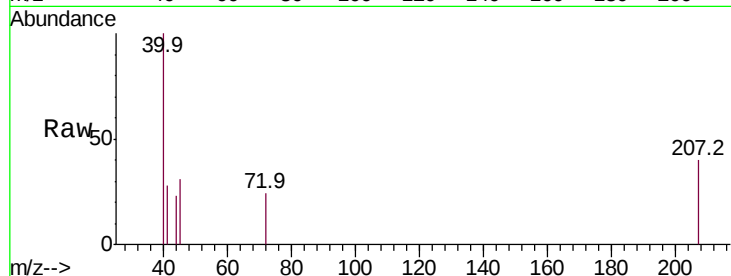


Abundance Ion 41.00 (40.70 to 41.70): VDC
Ion 39.00 (38.70 to 39.70): VDC
Ion 67.00 (66.70 to 67.70): VDC
Ion 52.00 (51.70 to 52.70): VDC


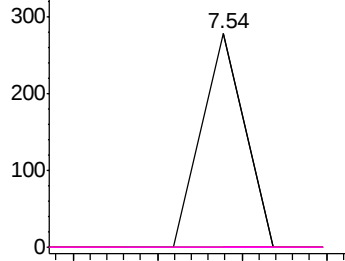



#48
Methyl methacrylate
Concen: 9.652 ug/l
RT: 9.44 min Scan# 1278
Delta R.T. -0.02 min
Lab File: VD067607.D
Acq: 11 Nov 2020 17:25

Tgt Ion: 41 Resp: 1572
Ion Ratio Lower Upper
41 100
69 0.0 80.6 121.0#
39 47.4 50.2 75.4#



Abundance Ion 41.00 (40.70 to 41.70): VDC
Ion 69.00 (68.70 to 69.70): VDC
Ion 39.00 (38.70 to 39.70): VDC




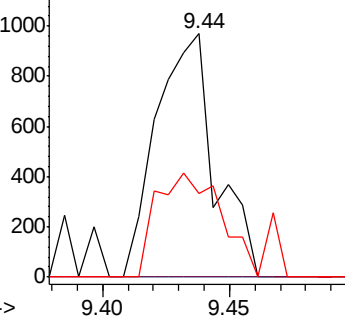


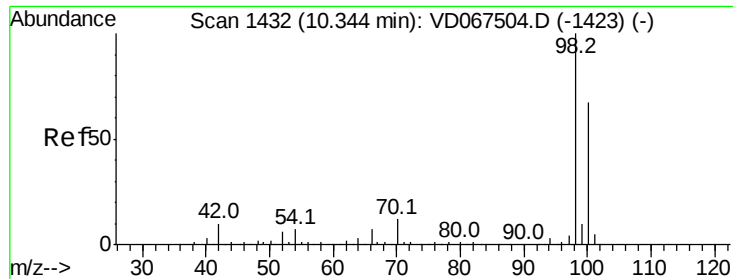

#50
Toluene-d8
Concen: 57.179 ug/l
RT: 10.34 min Scan# 1432
Delta R.T. -0.00 min
Lab File: VD067607.D
Acq: 11 Nov 2020 17:25




Instrument :
MSVOA_D
ClientSampleId :
16874


Tot Ion: 98 Resp: 86892
Ion Ratio Lower Upper
98 100
100 68.3 53.0 79.6

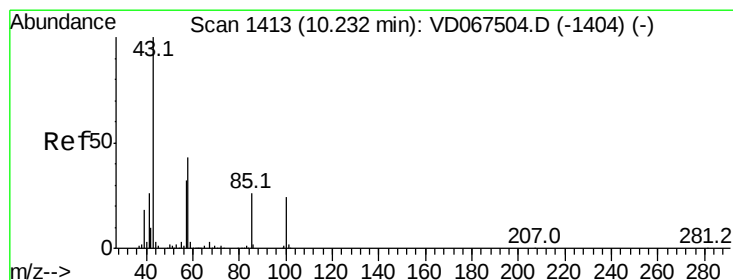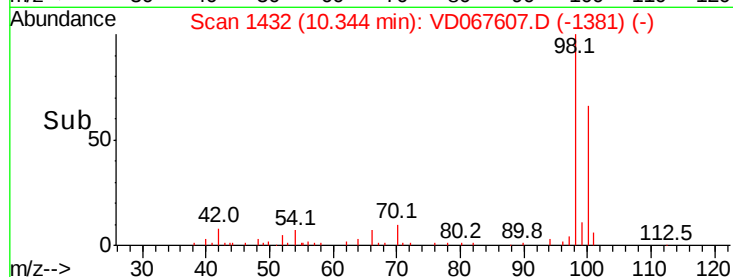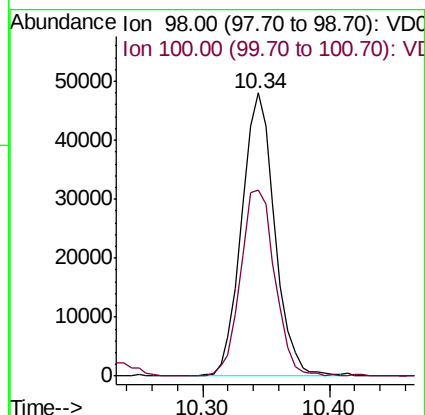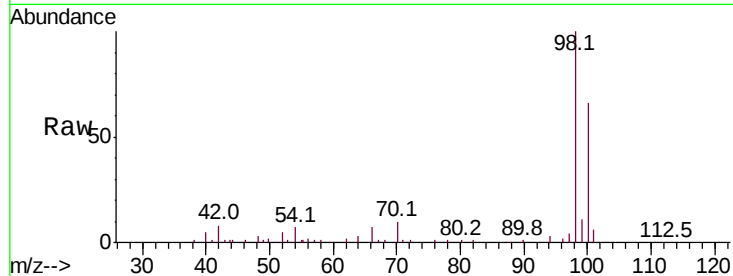

#51
4-Methyl-2-Pentanone
Concen: 122.909 ug/l
RT: 10.23 min Scan# 1412
Delta R.T. -0.01 min
Lab File: VD067607.D
Acq: 11 Nov 2020 17:25

Tgt Ion: 43 Resp: 18542
Ion Ratio Lower Upper
43 100
58 42.4 35.6 53.4

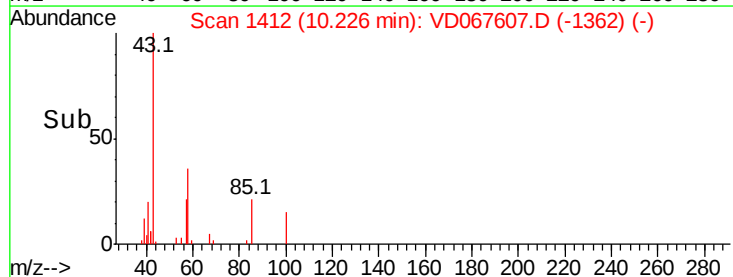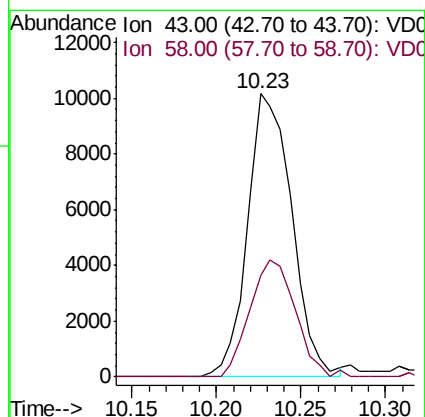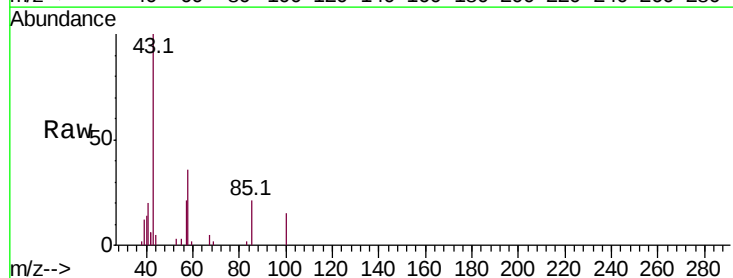



#52

Toluene

Concen: 5.960 ug/l

RT: 10.41 min Scan# 1444

Delta R.T. 0.01 min

Lab File: VD067607.D

Acq: 11 Nov 2020 17:25

Instrument :

MSVOA_D

ClientSampleId :





16874

Tot Ion: 92 Resp: 6643

Ion Ratio Lower Upper

92 100

91 181.9 137.0 205.6

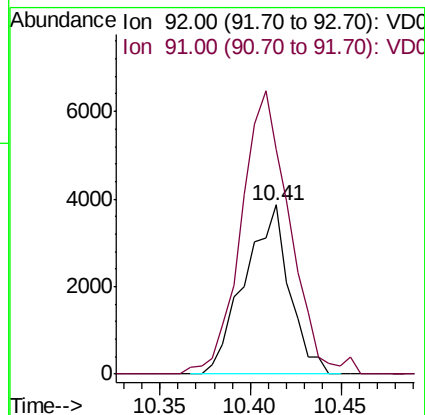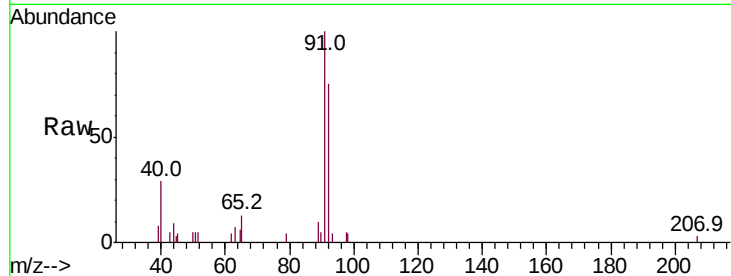

#56

Ethyl methacrylate

Concen: 1.286 ug/l

RT: 10.76 min Scan# 1503

Delta R.T. 0.09 min

Lab File: VD067607.D

Acq: 11 Nov 2020 17:25




Tgt Ion: 69 Resp: 402


Ion Ratio Lower Upper

69 100

41 628.9 45.4 68.0#

39 358.5 27.4 41.0#



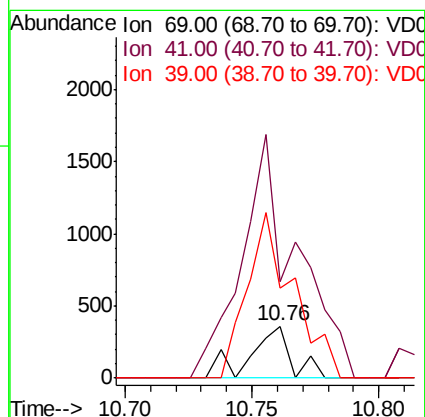



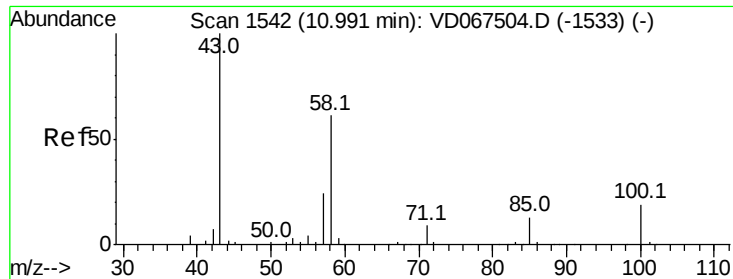

#59
2-Hexanone
Concen: 56.626 ug/l
RT: 10.98 min Scan# 1541
Delta R.T. -0.01 min
Lab File: VD067607.D
Acq: 11 Nov 2020 17:25




Instrument :
MSVOA_D
ClientSampleId :
16874


Tot Ion: 43 Resp: 5973
Ion Ratio Lower Upper
43 100
58 46.4 30.3 90.9

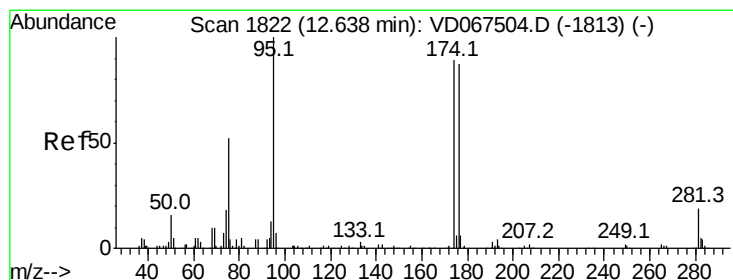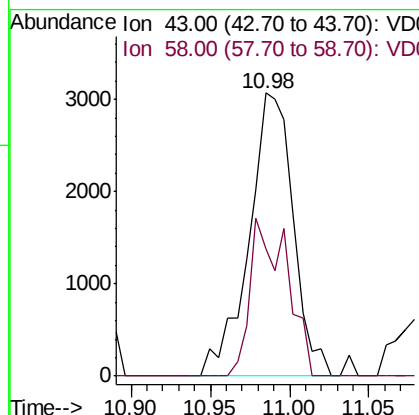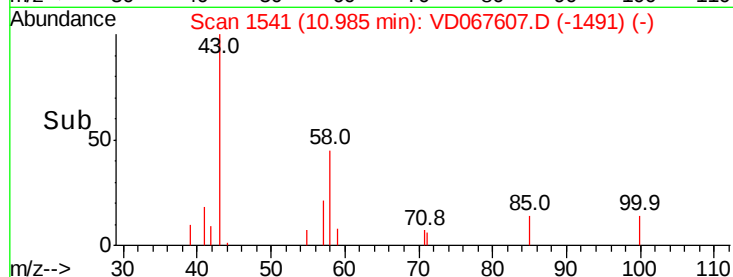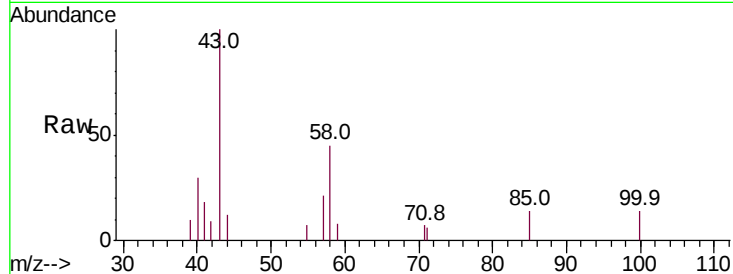

#62
4-Bromofluorobenzene
Concen: 71.070 ug/l
RT: 12.64 min Scan# 1822
Delta R.T. -0.00 min
Lab File: VD067607.D
Acq: 11 Nov 2020 17:25

Tgt Ion: 95 Resp: 37287
Ion Ratio Lower Upper
95 100
174 87.9 0.0 177.8
176 87.7 0.0 172.0


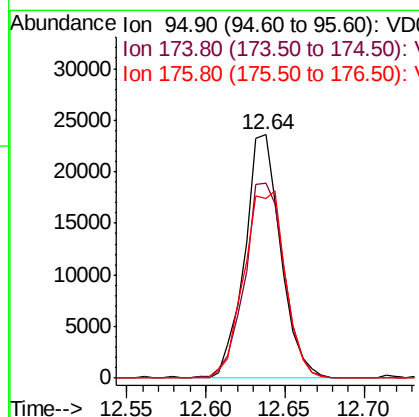
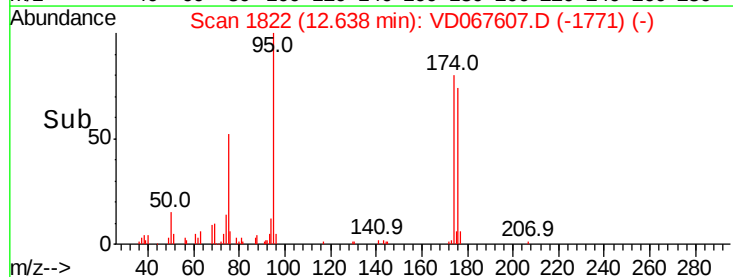
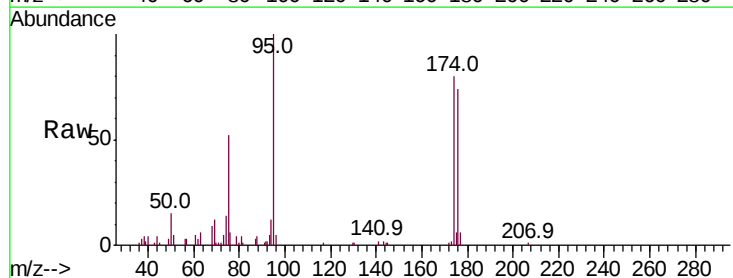




#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.65 min Scan# 1654
Delta R.T. -0.00 min
Lab File: VD067607.D
Acq: 11 Nov 2020 17:25




Instrument :
MSVOA_D
ClientSampleId :
16874


Tot Ion:117 Resp: 79211
Ion Ratio Lower Upper
117 100
82 47.6 41.6 62.4
119 31.9 25.1 37.7

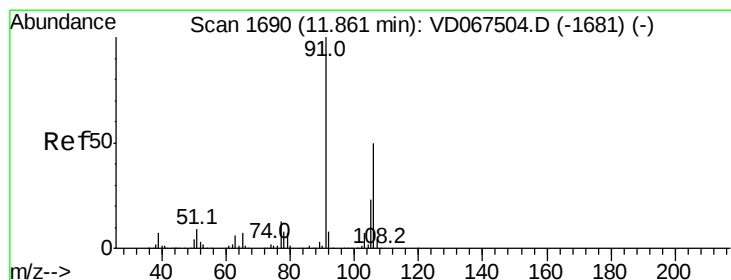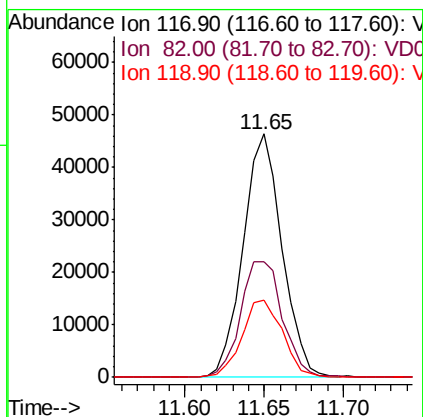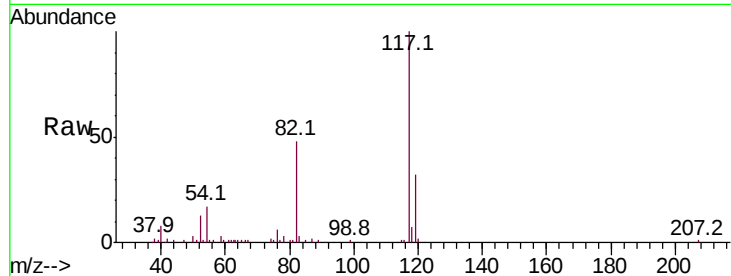

#68
m/p-Xylenes
Concen: 6.327 ug/l
RT: 11.86 min Scan# 1689
Delta R.T. -0.01 min
Lab File: VD067607.D
Acq: 11 Nov 2020 17:25

Tgt Ion:106 Resp: 6427
Ion Ratio Lower Upper
106 100
91 200.2 162.6 244.0



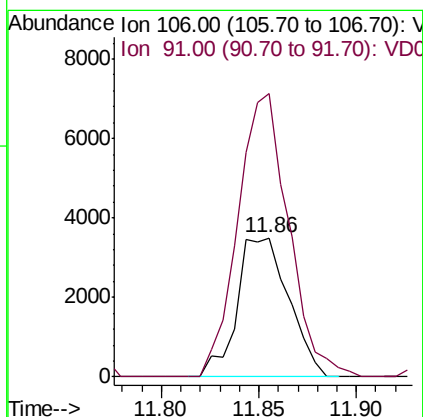





#69
o-Xylene
Concen: 12.431 ug/l
RT: 12.18 min Scan# 1744
Delta R.T. -0.01 min
Lab File: VD067607.D
Acq: 11 Nov 2020 17:25




Instrument :
MSVOA_D
ClientSampleId :
16874


Tot Ion:106 Resp: 11274
Ion Ratio Lower Upper
106 100
91 195.4 107.1 321.1

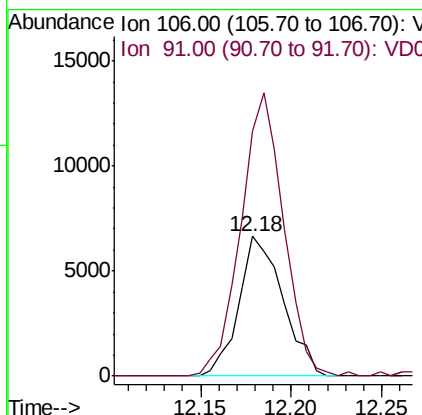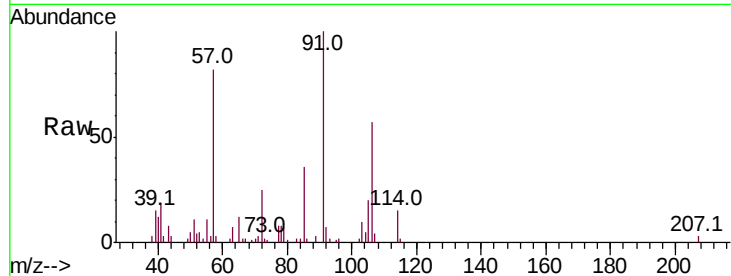

#71
Bromoform
Concen: 1.347 ug/l
RT: 12.64 min Scan# 1822
Delta R.T. 0.27 min
Lab File: VD067607.D
Acq: 11 Nov 2020 17:25

Tgt Ion:173 Resp: 413
Ion Ratio Lower Upper
173 100
175 0.0 24.1 72.2#
254 0.0 0.0 0.0

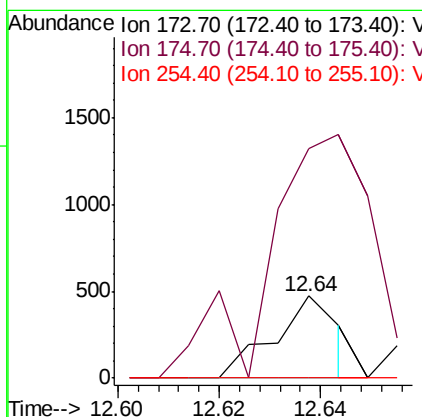

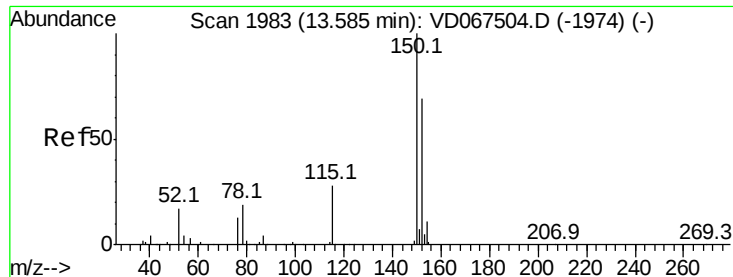

#72

1,4-Dichlorobenzene-d4

Concen: 50.000 ug/l

RT: 13.58 min Scan# 1982

Delta R.T. -0.01 min

Lab File: VD067607.D

Acq: 11 Nov 2020 17:25

Instrument :

MSVOA_D

ClientSampleId :

16874


Tot Ion:152 Resp: 39227

Ion Ratio Lower Upper

152 100

115 56.2 29.3 88.0




150 152.1 0.0 338.2

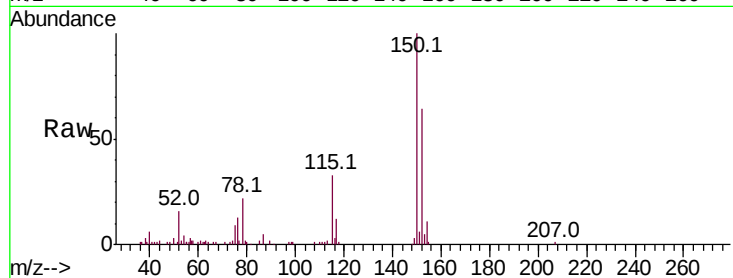

Abundance Ion 151.90 (151.60 to 152.60): V

Ion 114.90 (114.60 to 115.60): V

Ion 149.90 (149.60 to 150.60): V

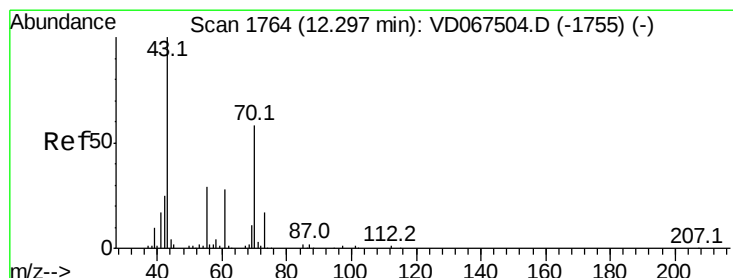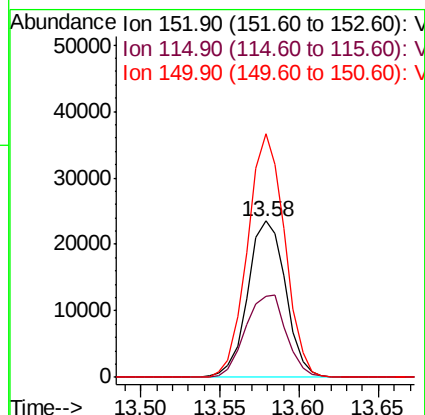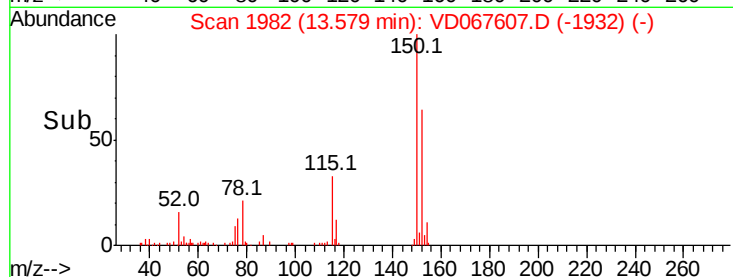

#74

N-ethyl acetate

Concen: 103.262 ug/l

RT: 12.26 min Scan# 1757

Delta R.T. -0.04 min

Lab File: VD067607.D

Acq: 11 Nov 2020 17:25

Tgt Ion: 43 Resp: 34447


Ion Ratio Lower Upper

43 100

70 0.7 42.6 64.0#

55 11.6 23.7 35.5#

61 0.0 21.9 32.9#


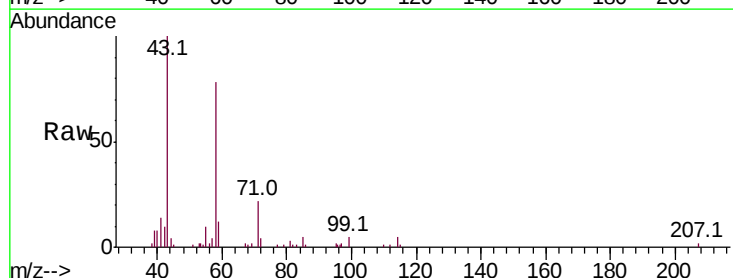



Abundance Ion 43.00 (42.70 to 43.70): VDC

Ion 70.00 (69.70 to 70.70): VDC

Ion 55.00 (54.70 to 55.70): VDC

Ion 61.00 (60.70 to 61.70): VDC

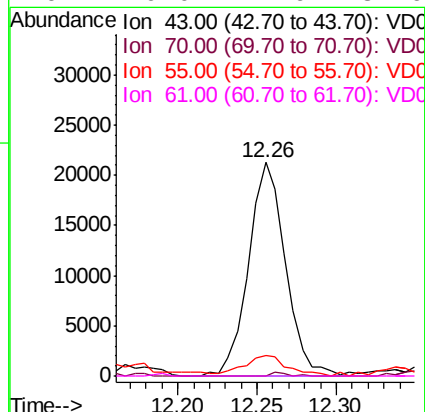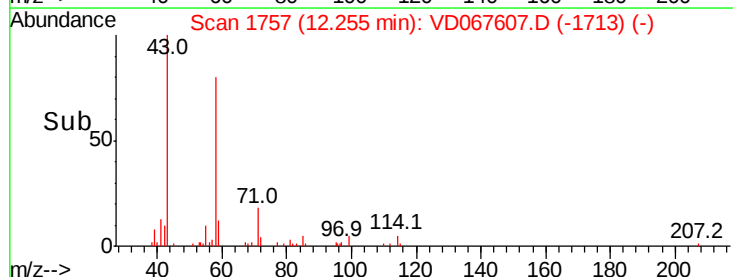



#75

1,1,2,2-Tetrachloroethane

Concen: 1.449 ug/l

RT: 12.76 min Scan# 1843

Delta R.T. 0.02 min

Lab File: VD067607.D

Acq: 11 Nov 2020 17:25

Instrument :

MSVOA_D

ClientSampleId :

16874


Tot Ion: 83 Resp: 501

Ion Ratio Lower Upper

83 100

131 0.0 7.1 21.3#

85 0.0 32.9 98.7#



Abundance Ion 82.90 (82.60 to 83.60): VDC
Ion 130.80 (130.50 to 131.50): VDC
Ion 84.90 (84.60 to 85.60): VDC



12.76

400

200

0

Time--> 12.72 12.74 12.76 12.78



#76

1,2,3-Trichloropropane

Concen: 81.461 ug/l

RT: 12.64 min Scan# 1822

Delta R.T. -0.15 min

Lab File: VD067607.D


Acq: 11 Nov 2020 17:25

Tgt Ion: 75 Resp: 19277

Ion Ratio Lower Upper

75 100

77 0.4 0.0 0.0#



Abundance Ion 74.90 (74.60 to 75.60): VDC
Ion 77.00 (76.70 to 77.70): VDC


12.64


10000

5000

0

Time--> 12.60 12.65 12.70





#81

trans-1,4-Dichloro-2-butene

Concen: 5.620 ug/l

RT: 12.47 min Scan# 1793

Delta R.T. -0.06 min

Lab File: VD067607.D

Acq: 11 Nov 2020 17:25

Instrument :

MSVOA_D

ClientSampleId :

16874


Tot Ion: 75 Resp: 655

Ion Ratio Lower Upper

75 100

53 21.7 75.9 113.9#




89 0.0 44.6 67.0#

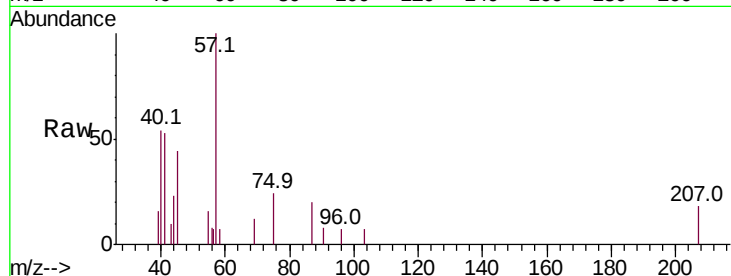

Abundance Ion 74.90 (74.60 to 75.60): VDC

Ion 53.00 (52.70 to 53.70): VDC

Ion 88.90 (88.60 to 89.60): VDC

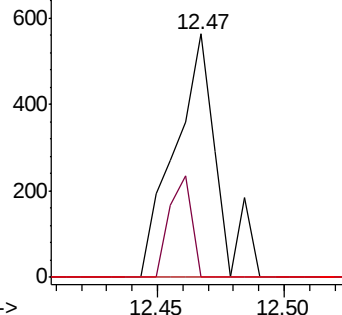

#84

1,2,4-Trimethylbenzene

Concen: 1.212 ug/l

RT: 13.27 min Scan# 1930

Delta R.T. -0.00 min

Lab File: VD067607.D


Acq: 11 Nov 2020 17:25

Tgt Ion: 105 Resp: 2612

Ion Ratio Lower Upper



105 100


120 53.3 22.1 66.1



Abundance Ion 105.00 (104.70 to 105.70): V

Ion 120.00 (119.70 to 120.70): V

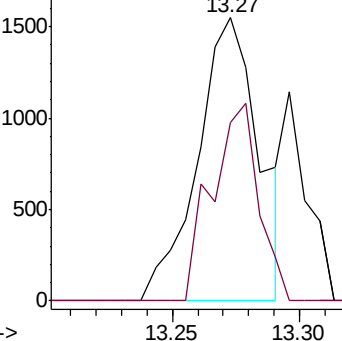

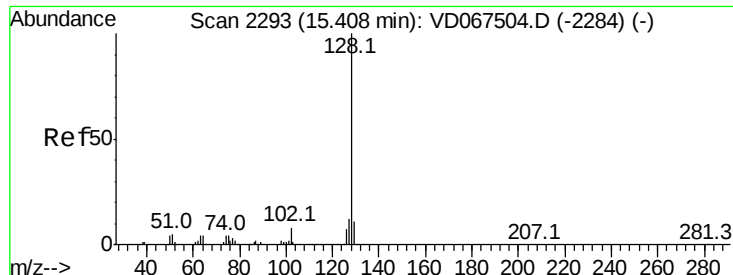

#95

Naphthalene

Concen: 2.381 ug/l

RT: 15.41 min Scan# 2294

Delta R.T. 0.01 min

Lab File: VD067607.D

Acq: 11 Nov 2020 17:25

Instrument :

MSVOA_D

ClientSampleId :

16874

Tot Ion:128 Resp: 2564

Ion Ratio Lower Upper

128 100

127 5.7 10.2 15.4#

129 0.0 8.9 13.3#

