


Data Path : Z:\voasrv\HPCHEM1\MSVOA D\Data\VD111720\
 Data File : VD067650.D
 Acq On : 17 Nov 2020 09:22
 Operator : VA/SY
 Sample : BFB
 Misc : 5.00G/5.00ml/MSVOA D/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_D
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_D\METHOD\82D110320S.M
 Title : SW846 8260
 Last Update : Wed Nov 04 00:56:28 2020

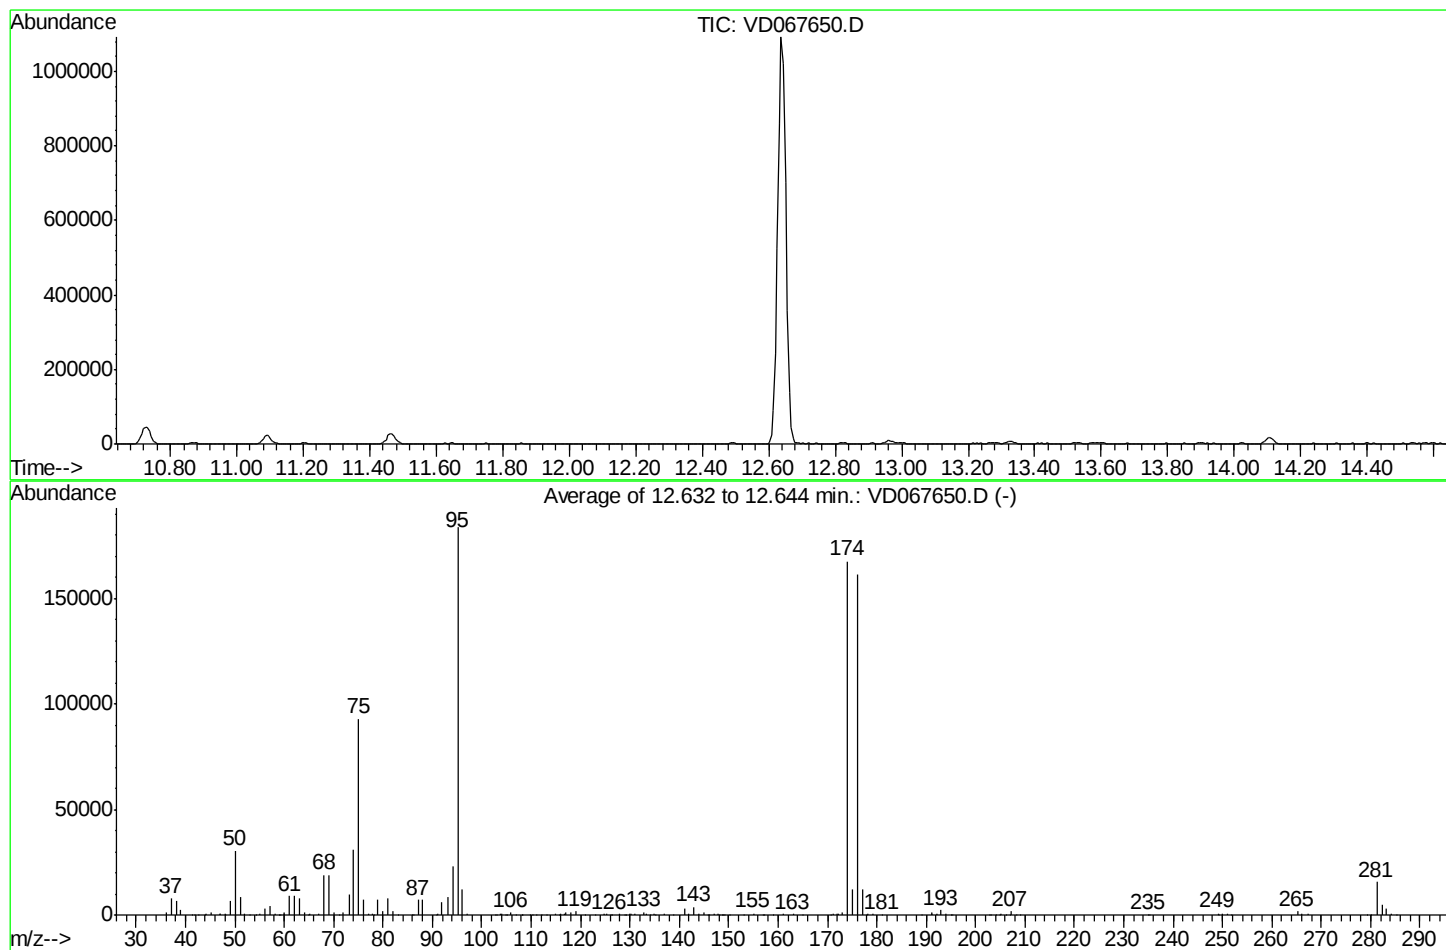

AutoFind: Scans 1821, 1822, 1823; Background Corrected with Scan 1812

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.6	30426	PASS
75	95	30	60	50.6	92829	PASS
95	95	100	100	100.0	183616	PASS
96	95	5	9	6.6	12063	PASS
173	174	0.00	2	0.9	1528	PASS
174	95	50	100	91.3	167637	PASS
175	174	5	9	7.4	12436	PASS
176	174	95	101	96.1	161173	PASS
177	176	5	9	7.4	11955	PASS