

Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD111825\
 Data File : VD080532.D
 Acq On : 18 Nov 2025 10:37
 Operator : RP/MD
 Sample : VD1118SBL01
 Misc : 5.00G/5ml/MSVOA_D/SOIL
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_D
 ClientSampleId :
 VD1118SBL01

Quant Time: Nov 18 11:35:13 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D111725S.M
 Quant Title : SW846 8260
 QLast Update : Tue Nov 18 00:45:54 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	7.876	168	297421	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	8.776	114	489620	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.582	117	408840	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.517	152	177899	50.000	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.229	65	118300	47.371	ug/l	0.00
Spiked Amount	50.000	Range	50 - 163	Recovery	=	94.740%
35) Dibromofluoromethane	7.806	113	140095	48.602	ug/l	0.00
Spiked Amount	50.000	Range	54 - 147	Recovery	=	97.200%
50) Toluene-d8	10.270	98	559255	47.960	ug/l	0.00
Spiked Amount	50.000	Range	58 - 134	Recovery	=	95.920%
62) 4-Bromofluorobenzene	12.570	95	159796	47.666	ug/l	0.00
Spiked Amount	50.000	Range	30 - 143	Recovery	=	95.340%


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD111825\
Data File : VD080532.D
Acq On : 18 Nov 2025 10:37
Operator : RP/MD
Sample : VD1118SBL01
Misc : 5.00G/5ml/MSVOA_D/SOIL
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
VD1118SBL01

Quant Time: Nov 18 11:35:13 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D111725S.M
Quant Title : SW846 8260
QLast Update : Tue Nov 18 00:45:54 2025
Response via : Initial Calibration




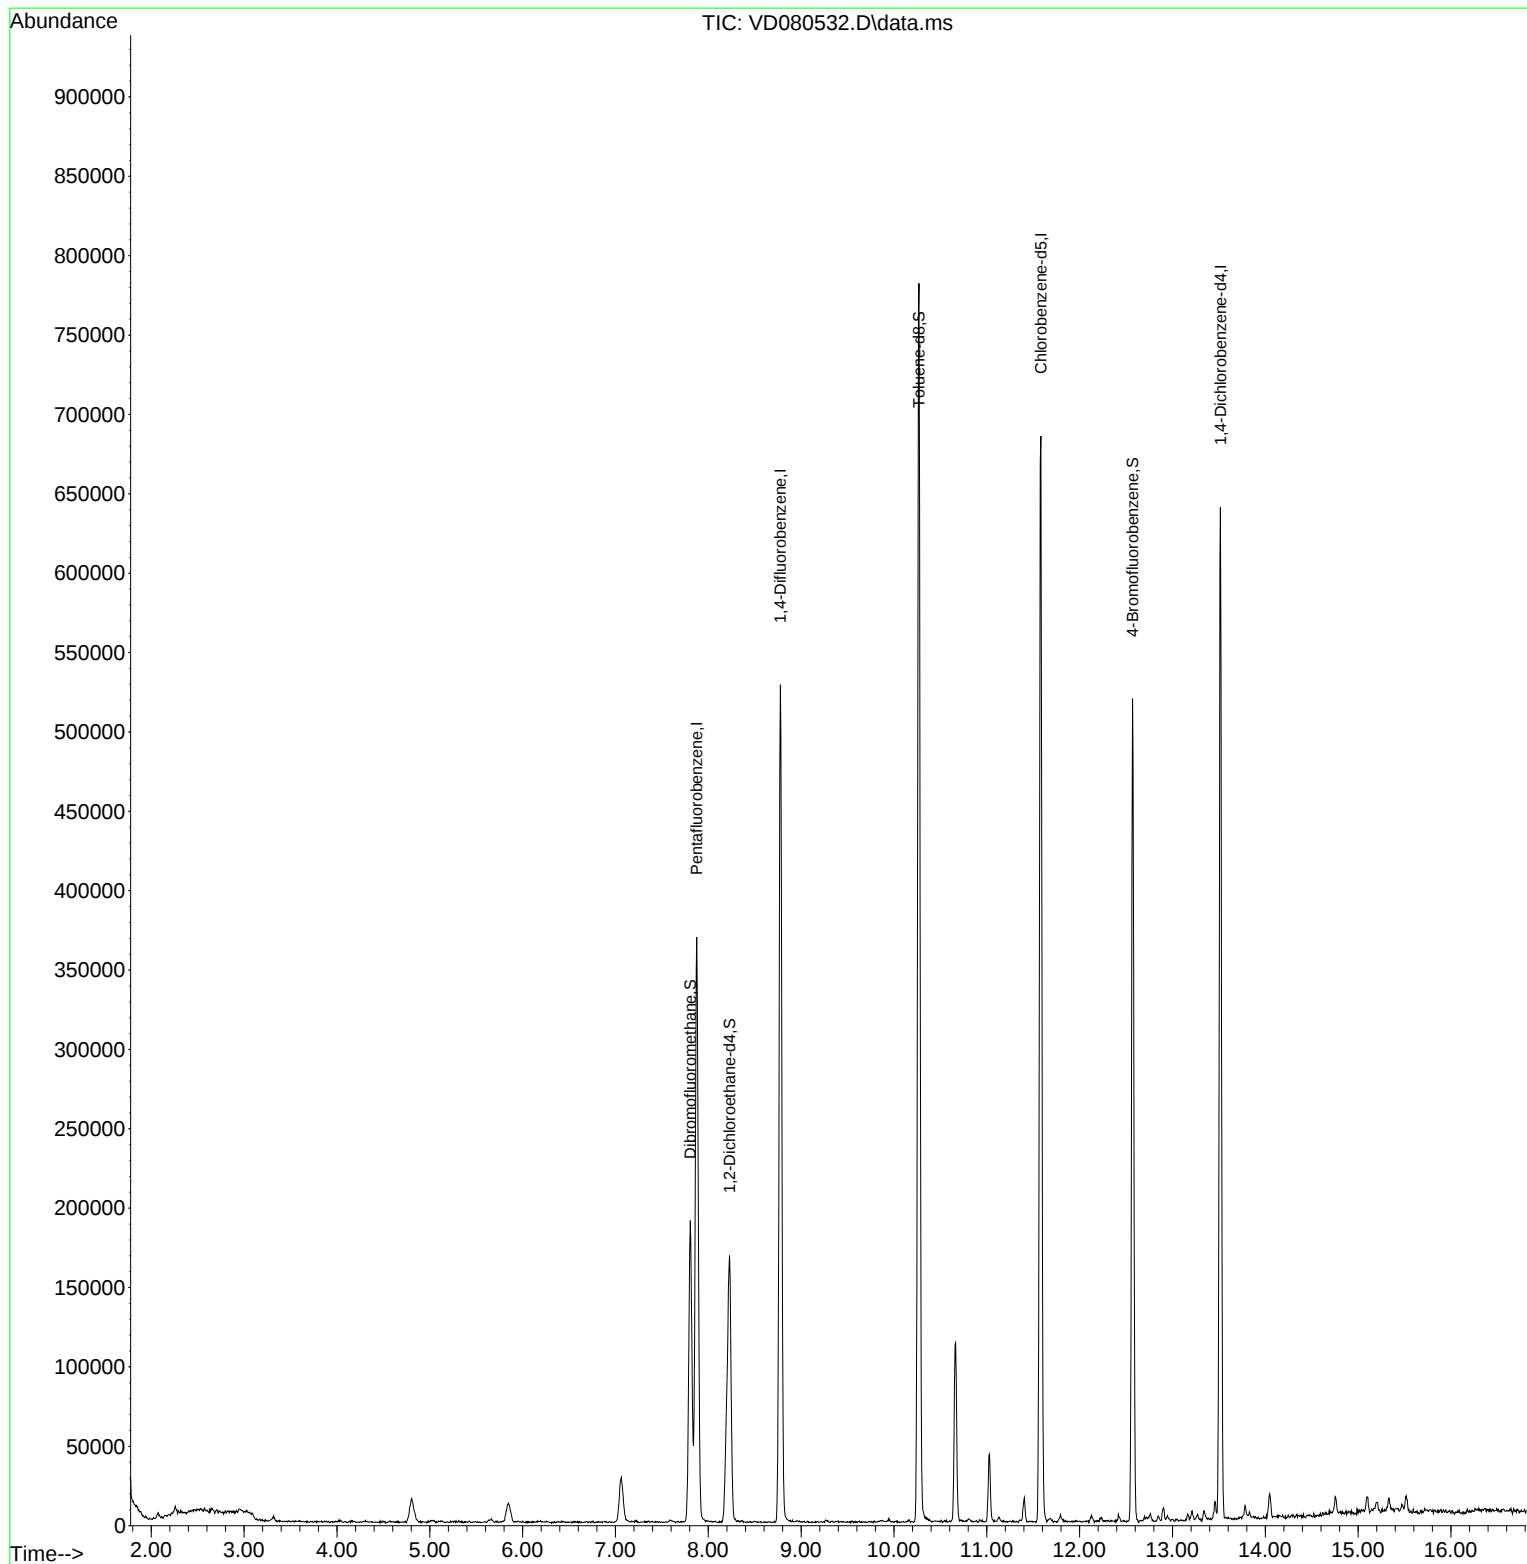


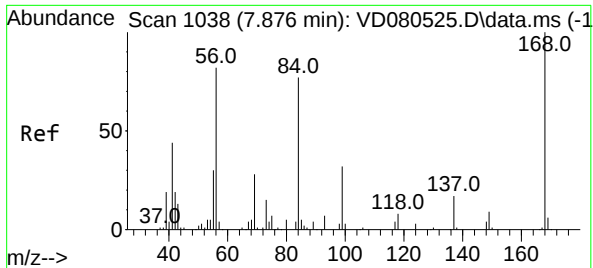

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 7.876 min Scan# 1038
Delta R.T. 0.000 min
Lab File: VD080532.D
Acq: 18 Nov 2025 10:37




Instrument :
MSVOA_D
ClientSampleId :
VD1118SBL01


Tgt Ion:168 Resp: 297421
Ion Ratio Lower Upper
168 100
99 56.8 42.5 63.7

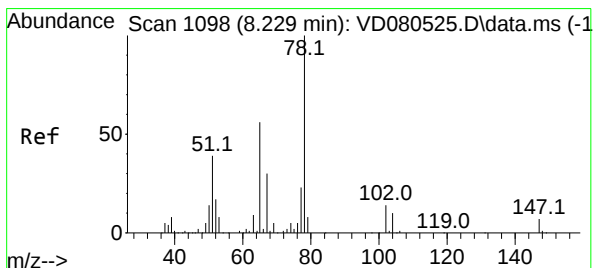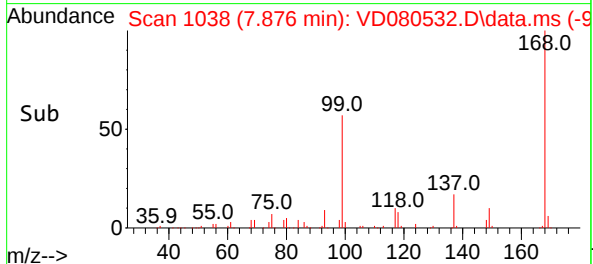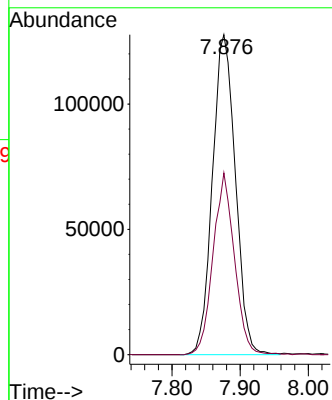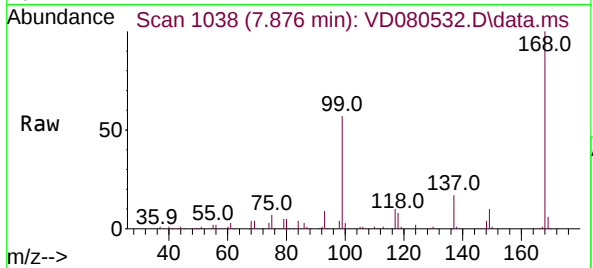

#33
1,2-Dichloroethane-d4
Concen: 47.371 ug/l
RT: 8.229 min Scan# 1098
Delta R.T. 0.000 min
Lab File: VD080532.D
Acq: 18 Nov 2025 10:37

Tgt Ion: 65 Resp: 118300
Ion Ratio Lower Upper
65 100
67 56.3 0.0 109.6

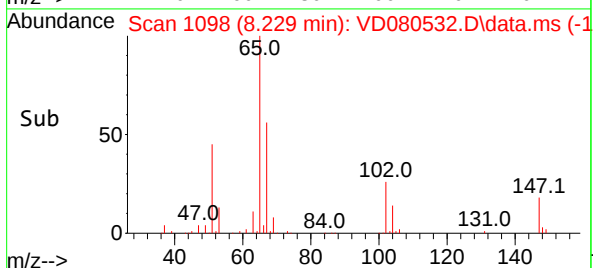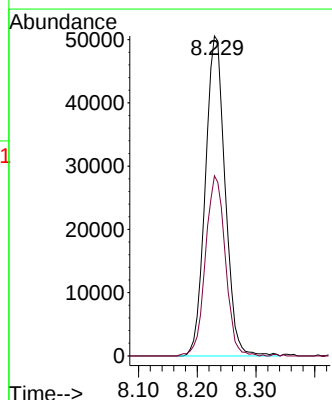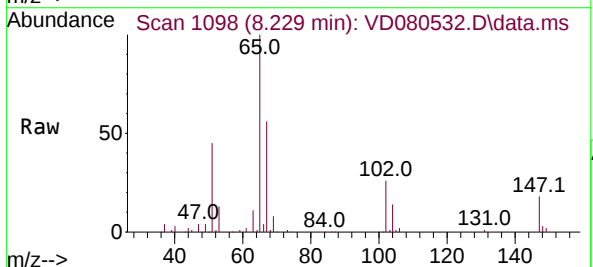

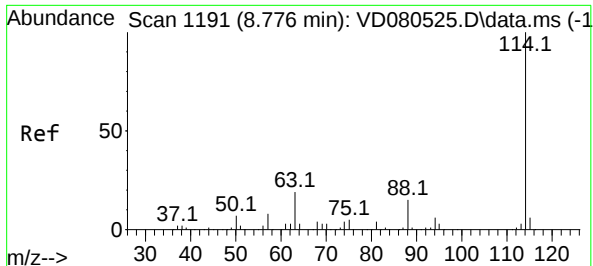

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 8.776 min Scan# 1191

Delta R.T. 0.000 min

Lab File: VD080532.D

Acq: 18 Nov 2025 10:37

Instrument :

MSVOA_D

ClientSampleId :

VD1118SBL01





Tgt Ion:114 Resp: 489620

Ion Ratio Lower Upper

114 100

63 19.7 0.0 38.2

88 13.8 0.0 29.6

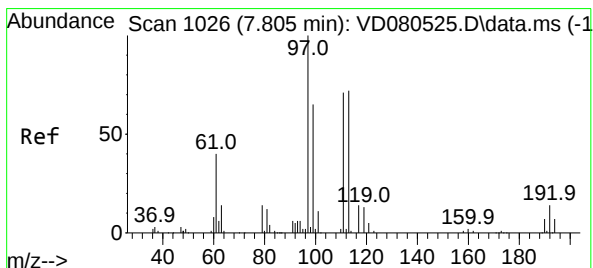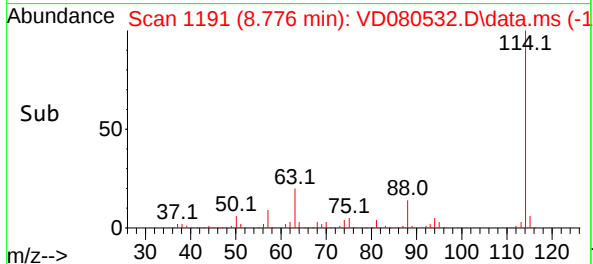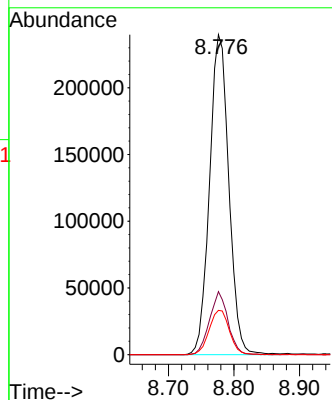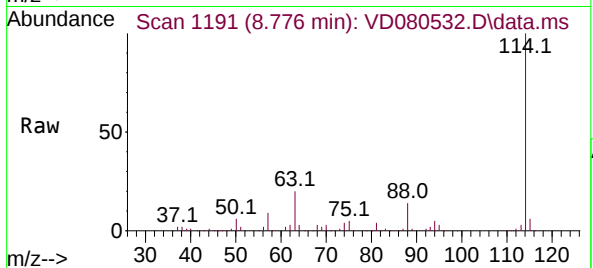

#35

Dibromofluoromethane

Concen: 48.602 ug/l

RT: 7.806 min Scan# 1026

Delta R.T. 0.000 min

Lab File: VD080532.D

Acq: 18 Nov 2025 10:37




Tgt Ion:113 Resp: 140095


Ion Ratio Lower Upper

113 100

111 101.1 82.2 123.2

192 19.8 16.0 24.0


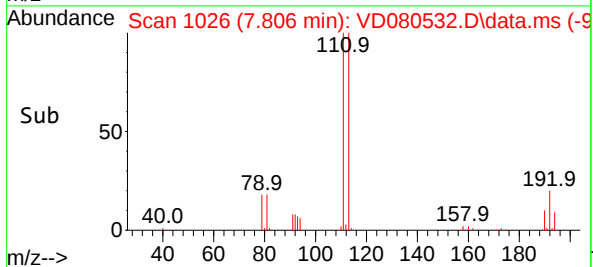
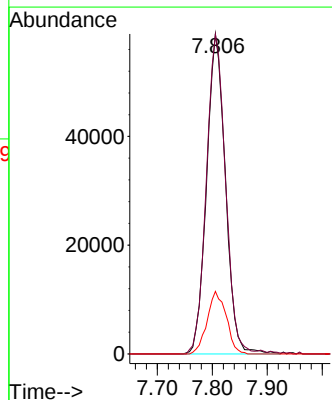
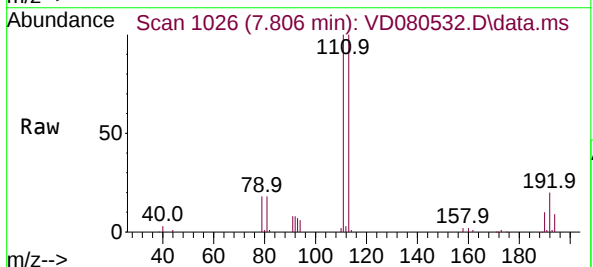


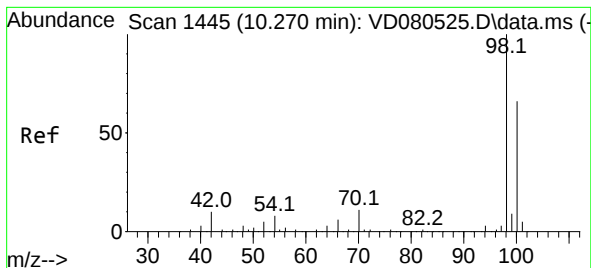

#50
Toluene-d8
Concen: 47.960 ug/l
RT: 10.270 min Scan# 1445
Delta R.T. 0.000 min
Lab File: VD080532.D
Acq: 18 Nov 2025 10:37




Instrument :
MSVOA_D
ClientSampleId :
VD1118SBL01


Tgt Ion: 98 Resp: 559255
Ion Ratio Lower Upper
98 100
100 65.3 52.0 78.0

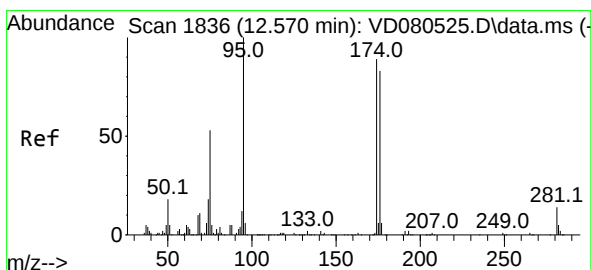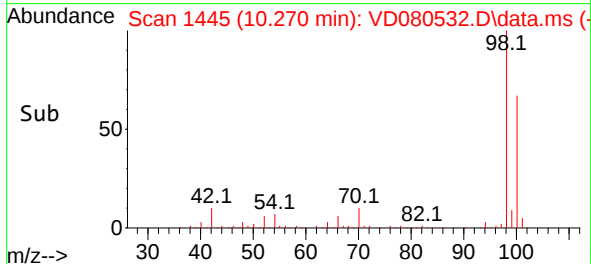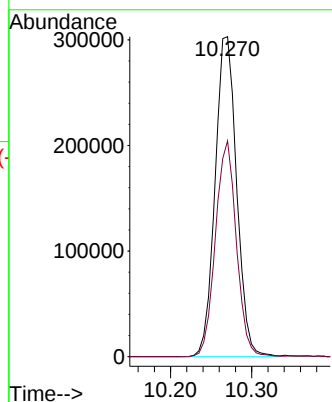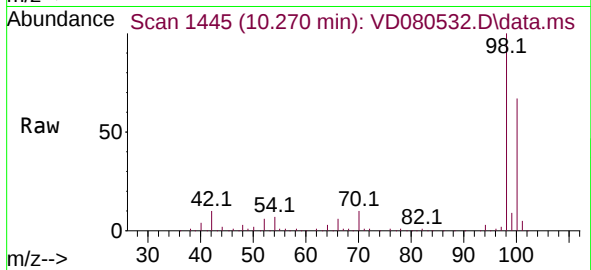

#62
4-Bromofluorobenzene
Concen: 47.666 ug/l
RT: 12.570 min Scan# 1836
Delta R.T. 0.000 min
Lab File: VD080532.D
Acq: 18 Nov 2025 10:37

Tgt Ion: 95 Resp: 159796
Ion Ratio Lower Upper
95 100
174 86.9 0.0 179.4
176 84.4 0.0 168.6


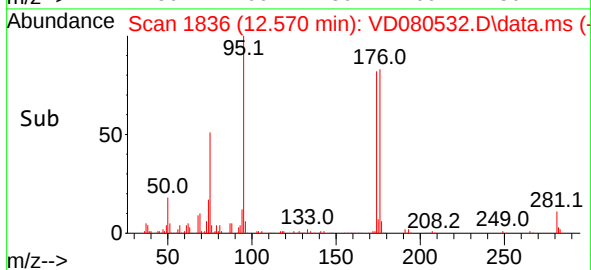
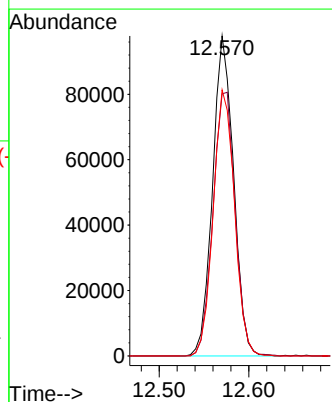
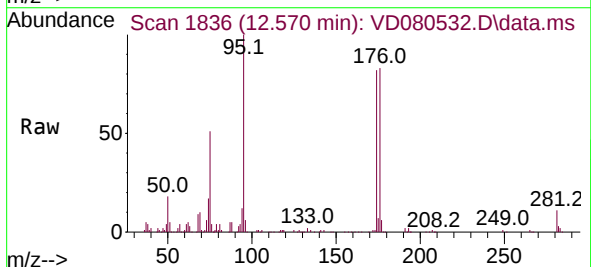


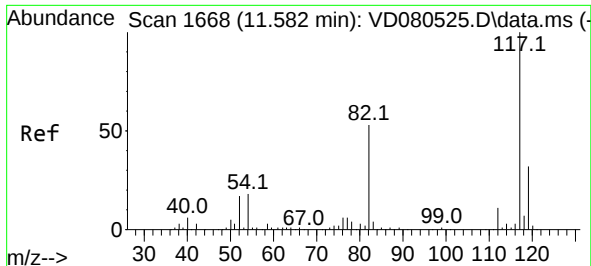

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.582 min Scan# 1668
Delta R.T. 0.000 min
Lab File: VD080532.D
Acq: 18 Nov 2025 10:37

Instrument :
MSVOA_D
ClientSampleId :
VD1118SBL01

Tgt Ion:117 Resp: 408840
Ion Ratio Lower Upper
117 100
82 53.5 42.1 63.1
119 31.4 25.4 38.2

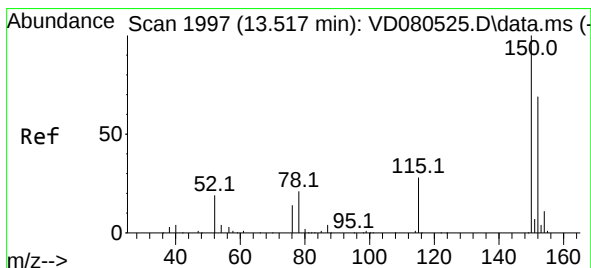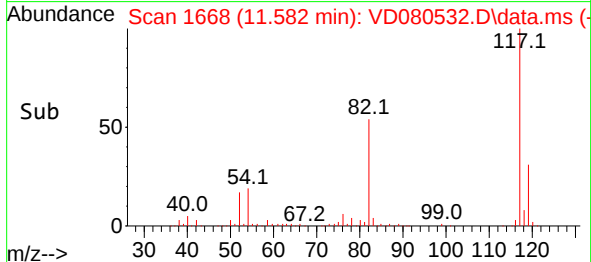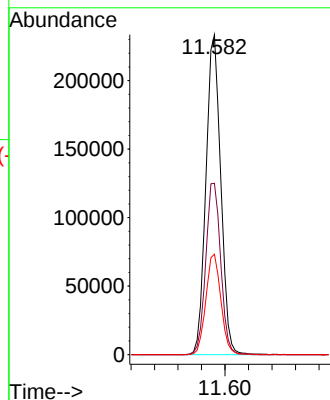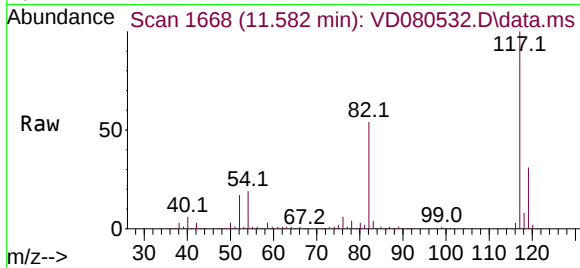

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.517 min Scan# 1997
Delta R.T. 0.000 min
Lab File: VD080532.D
Acq: 18 Nov 2025 10:37

Tgt Ion:152 Resp: 177899
Ion Ratio Lower Upper
152 100
115 57.4 28.1 84.3
150 159.1 0.0 345.6

