
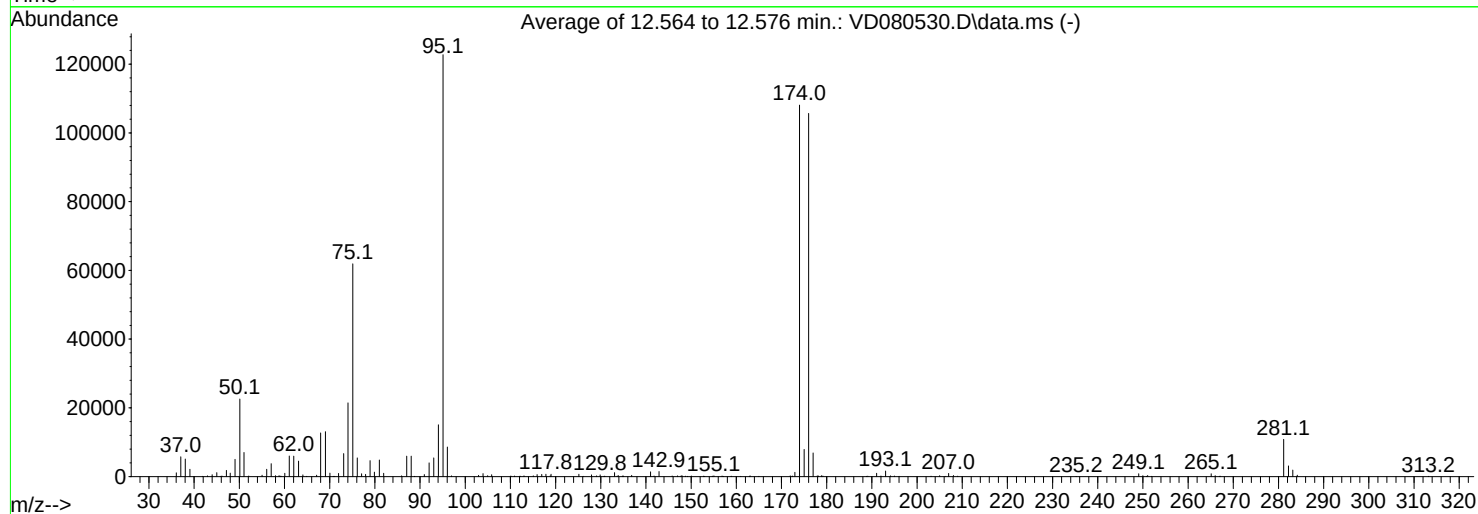


Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD111825\
Data File : VD080530.D
Acq On : 18 Nov 2025 08:19
Operator : RP/MD
Sample : BFB
Misc : 5.00G/5ml/MSVOA_D/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D111725S.M
Title : SW846 8260
Last Update : Tue Nov 18 00:45:54 2025

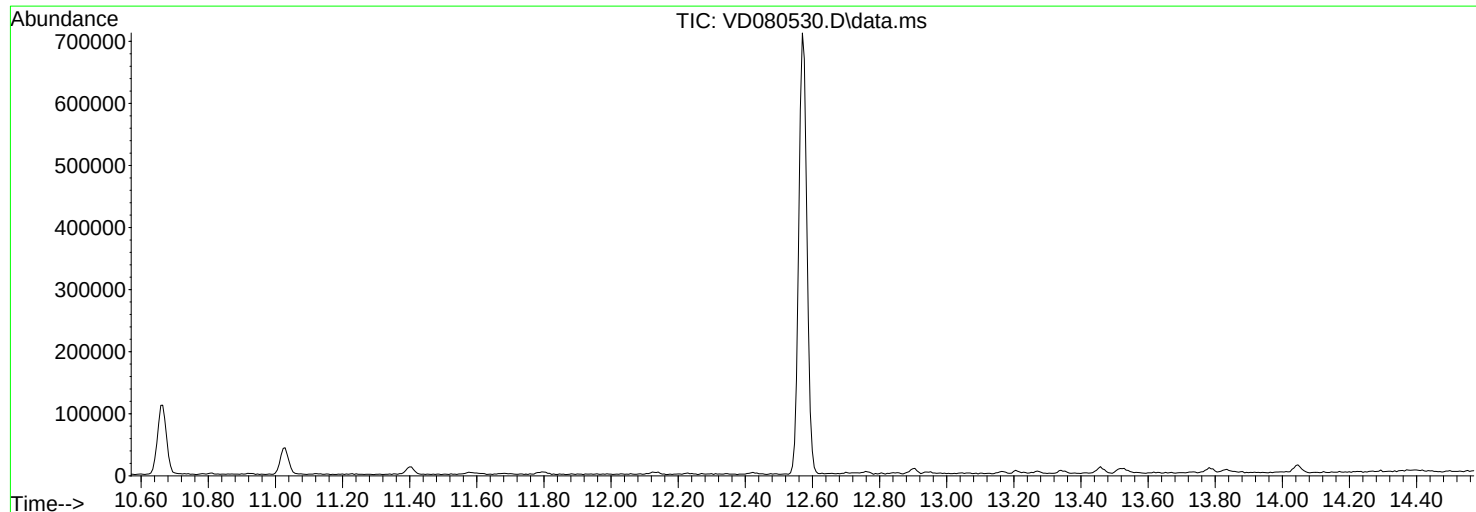

AutoFind: Scans 1835, 1836, 1837; Background Corrected with Scan 1827

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.4	22560	PASS
75	95	30	60	50.4	61915	PASS
95	95	100	100	100.0	122749	PASS
96	95	5	9	7.0	8597	PASS
173	174	0.00	2	1.2	1251	PASS
174	95	50	100	88.1	108088	PASS
175	174	5	9	7.3	7910	PASS
176	174	95	101	97.8	105659	PASS
177	176	5	9	6.5	6890	PASS