


Data Path : Z:\voasrv\HPCHEM1\MSVOA D\Data\VD111919\
Data File : VD064279.D
Acq On : 19 Nov 2019 09:44
Operator : VA/SY
Sample : BFB
Misc : 5.00G/5.00ml/MSVOA D/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_D\METHOD\82D110819S.M
Title : SW846 8260
Last Update : Tue Nov 12 02:43:24 2019

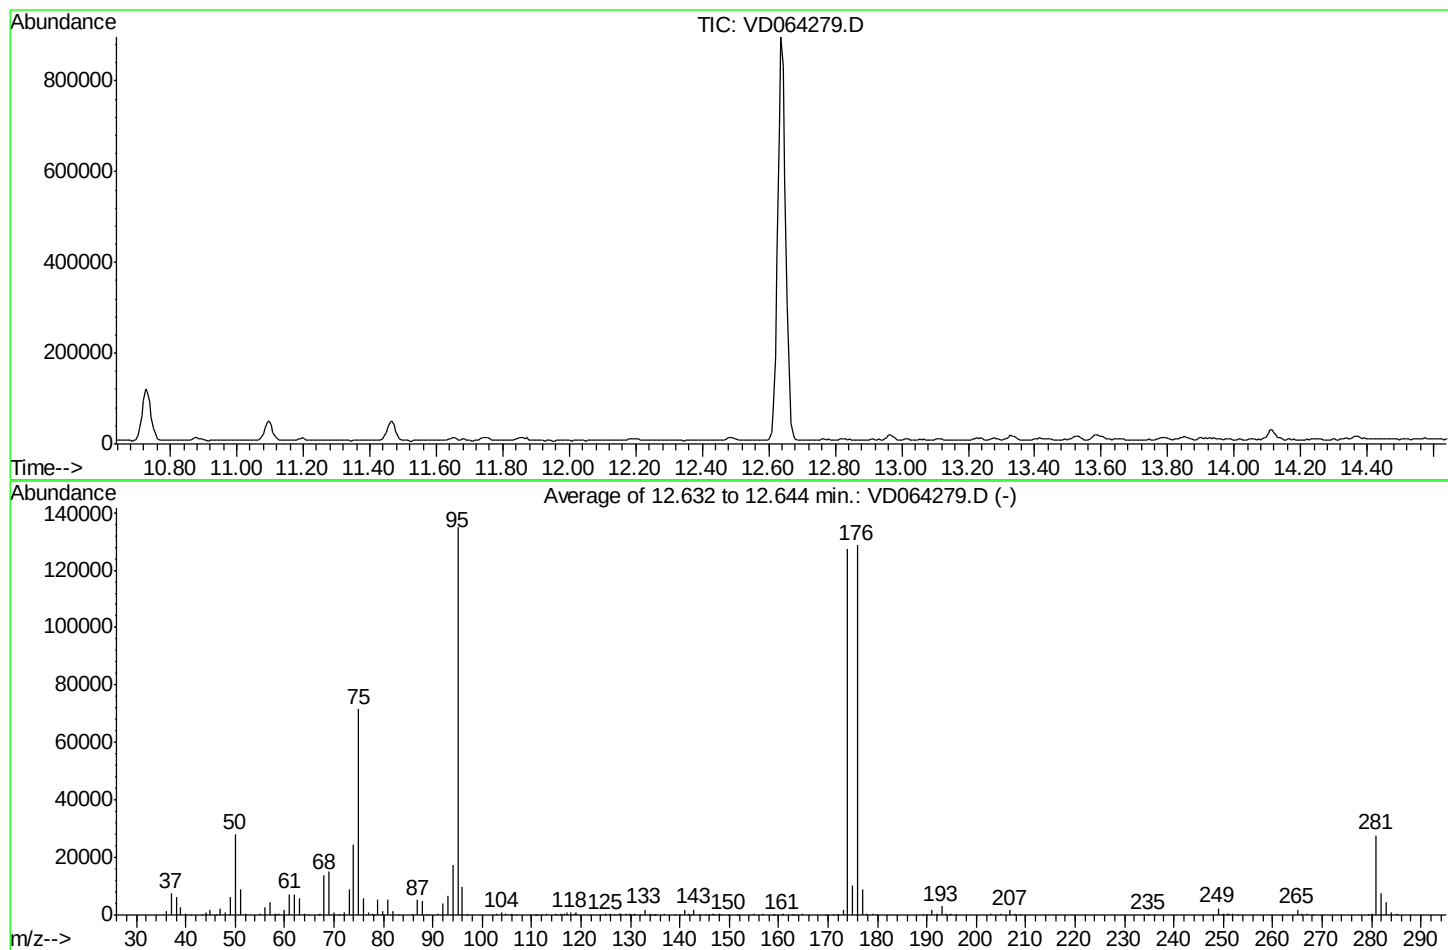

AutoFind: Scans 1821, 1822, 1823; Background Corrected with Scan 1812

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.8	28021	PASS
75	95	30	60	53.0	71522	PASS
95	95	100	100	100.0	134864	PASS
96	95	5	9	7.2	9668	PASS
173	174	0.00	2	1.5	1957	PASS
174	95	50	100	94.5	127418	PASS
175	174	5	9	8.1	10374	PASS
176	174	95	101	100.9	128568	PASS
177	176	5	9	7.0	9032	PASS