

Data Path : Z:\VOASRV\HPCHEM1\MSVOA D\DATA\VD120419\
 Data File : VD064416.D
 Acq On : 04 Dec 2019 14:52
 Operator : VA/SY
 Sample : K6119-03RE
 Misc : 4.69G/5.00ml/MSVOA D/SOIL
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_D
 ClientSampleId :
 SB-6-(1-3)RE

Quant Time: Dec 05 06:17:05 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_D\METHOD\82D112719S.M
 Quant Title : SW846 8260
 QLast Update : Fri Nov 29 07:18:03 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	7.97	168	13876	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	8.87	114	23632	50.00	ug/l	0.00
63) Chlorobenzene-d5	11.65	117	22467	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.58	152	11772	50.00	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.33	65	9569	76.19	ug/l	0.00
Spiked Amount	50.000		Recovery	=	152.38%	
35) Dibromofluoromethane	7.92	113	7196	48.33	ug/l	0.00
Spiked Amount	50.000		Recovery	=	96.66%	
50) Toluene-d8	10.34	98	27762	49.50	ug/l	0.00
Spiked Amount	50.000		Recovery	=	99.00%	
62) 4-Bromofluorobenzene	12.64	95	10217	56.68	ug/l	0.00
Spiked Amount	50.000		Recovery	=	113.36%	


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA D\DATA\VD120419\
Data File : VD064416.D
Acq On : 04 Dec 2019 14:52
Operator : VA/SY
Sample : K6119-03RE
Misc : 4.69G/5.00ml/MSVOA D/SOIL
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
SB-6-(1-3)RE

Quant Time: Dec 05 06:17:05 2019
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_D\METHOD\82D112719S.M
Quant Title : SW846 8260
QLast Update : Fri Nov 29 07:18:03 2019
Response via : Initial Calibration

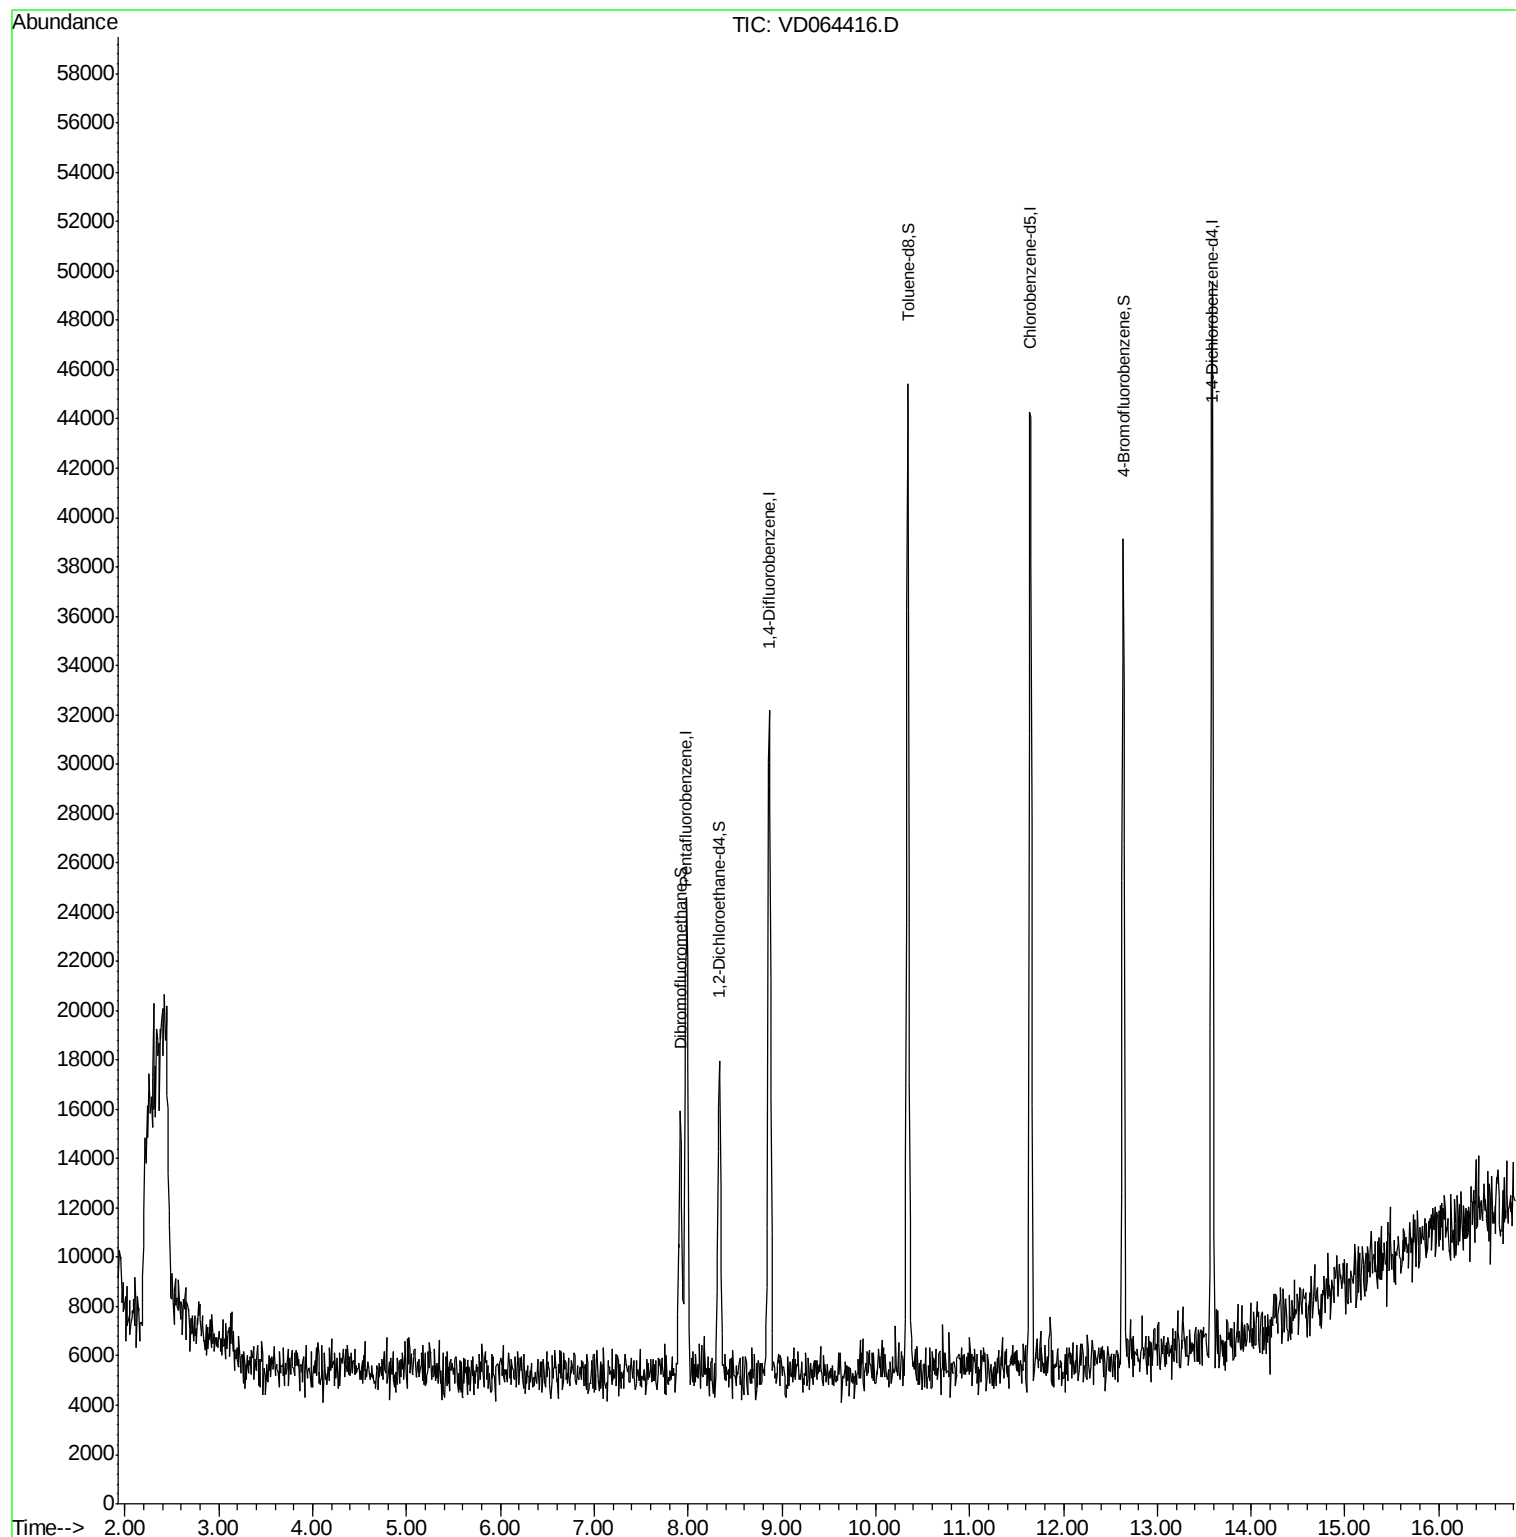

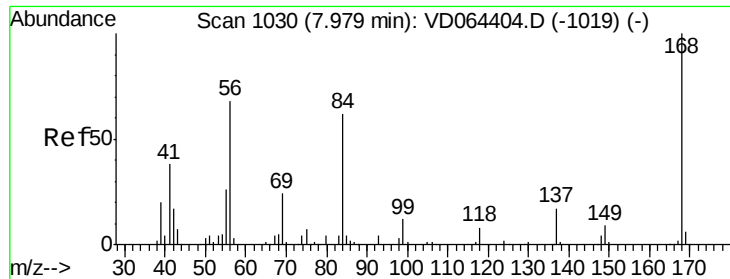

#1

Pentafluorobenzene

Concen: 50.000 ug/l

RT: 7.97 min Scan# 1029

Delta R.T. -0.01 min

Lab File: VD064416.D

Acq: 04 Dec 2019 14:52

Instrument :

MSVOA_D

ClientSampleId :


SB-6-(1-3)RE

Tot Ion:168 Resp: 13876

Ion Ratio Lower Upper




168 100

99 42.5 40.7 61.1

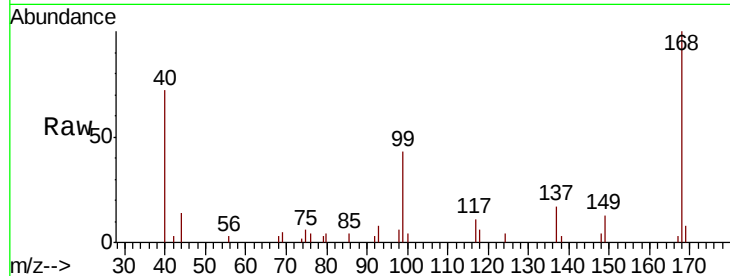

Abundance Ion 167.90 (167.60 to 168.60): V

Ion 98.90 (98.60 to 99.60): VDC

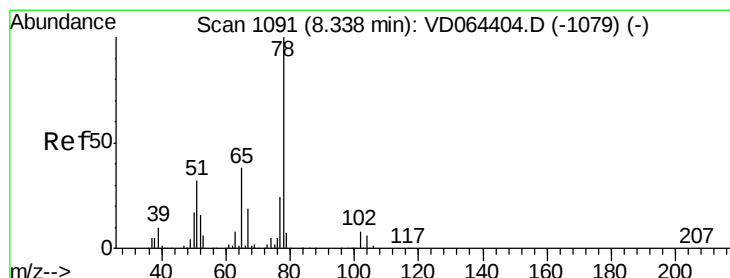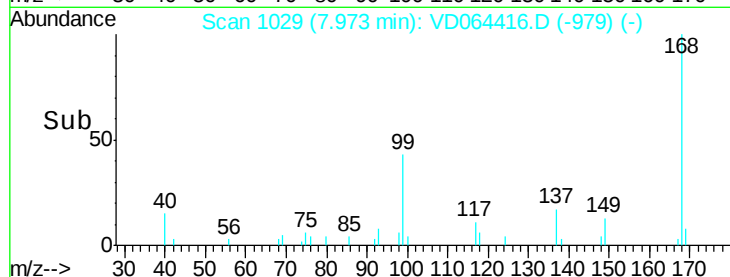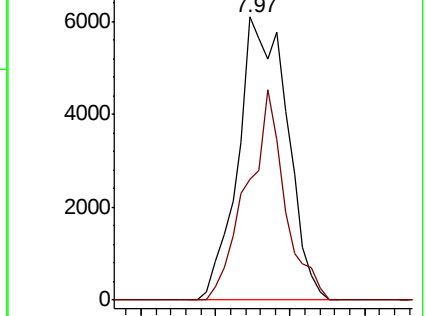

#33

1,2-Dichloroethane-d4

Concen: 76.187 ug/l

RT: 8.33 min Scan# 1090

Delta R.T. -0.01 min

Lab File: VD064416.D


Acq: 04 Dec 2019 14:52

Tgt Ion: 65 Resp: 9569

Ion Ratio Lower Upper



65 100


67 51.4 0.0 102.0

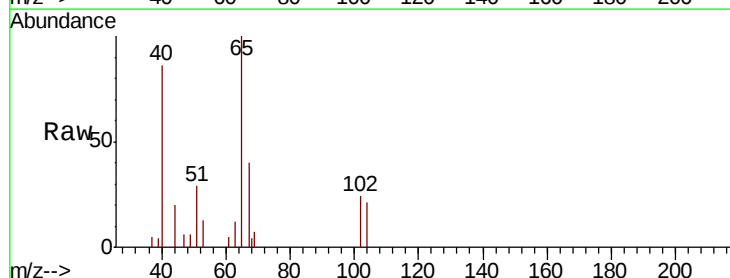

Abundance Ion 64.90 (64.60 to 65.60): VDC

Ion 66.90 (66.60 to 67.60): VDC

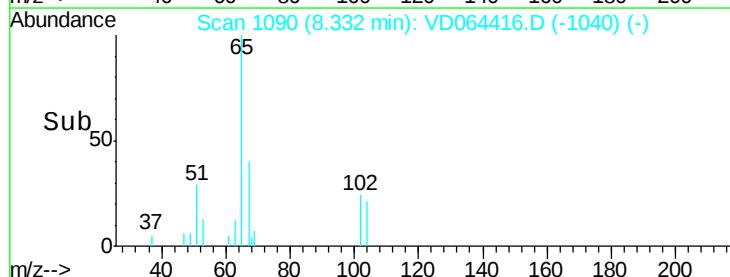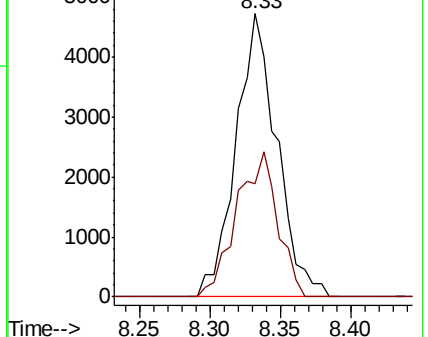

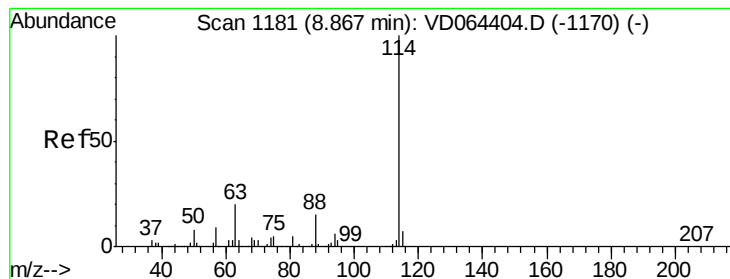

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 8.87 min Scan# 1181

Delta R.T. 0.00 min

Lab File: VD064416.D

Acq: 04 Dec 2019 14:52

Instrument :

MSVOA_D

ClientSampleId :

SB-6-(1-3)RE


Tot Ion:114 Resp: 23632

Ion Ratio Lower Upper

114 100

63 22.9 0.0 40.0




88 17.6 0.0 29.2

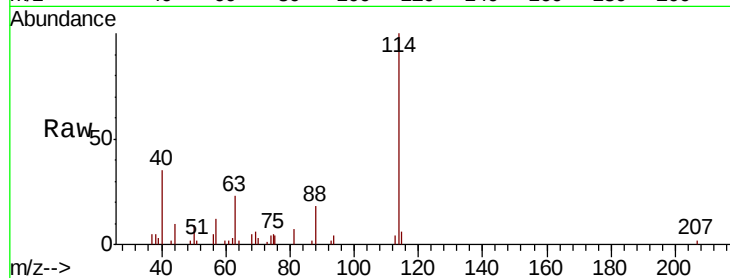

Abundance Ion 113.90 (113.60 to 114.60): V

Ion 63.00 (62.70 to 63.70): V

Ion 87.90 (87.60 to 88.60): V

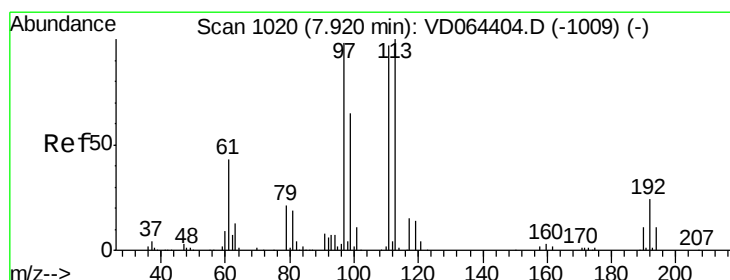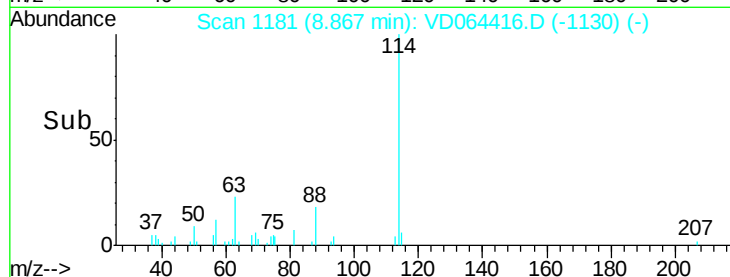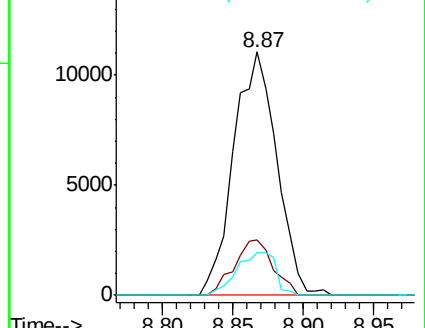

#35

Dibromofluoromethane

Concen: 48.330 ug/l

RT: 7.92 min Scan# 1020

Delta R.T. 0.00 min

Lab File: VD064416.D

Acq: 04 Dec 2019 14:52


Tgt Ion:113 Resp: 7196

Ion Ratio Lower Upper

113 100

111 105.4 79.4 119.2



192 22.9 18.6 28.0

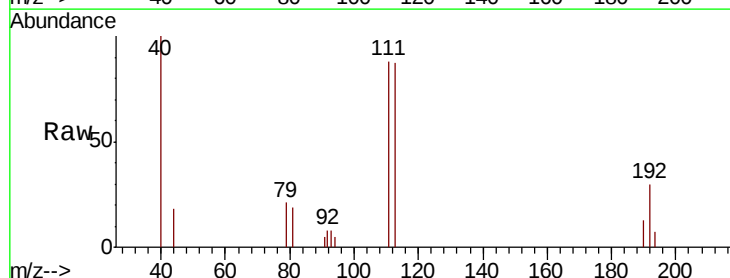

Abundance Ion 112.80 (112.50 to 113.50): V

Ion 110.80 (110.50 to 111.50): V

Ion 191.70 (191.40 to 192.40): V

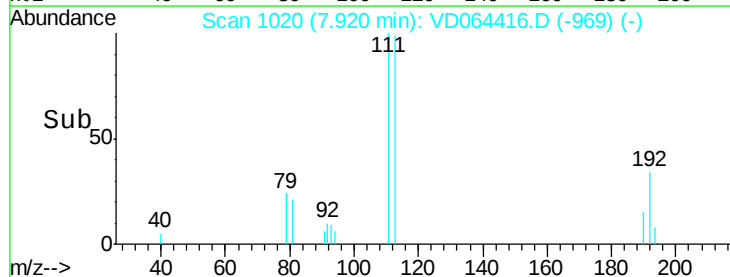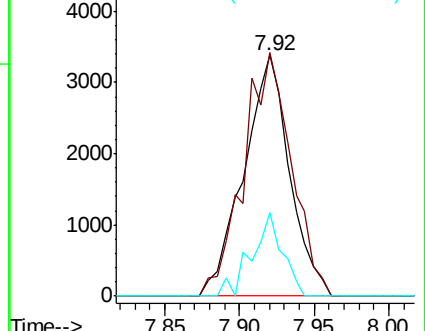



#50

Toluene-d8

Concen: 49.499 ug/l

RT: 10.34 min Scan# 1432

Delta R.T. 0.00 min

Lab File: VD064416.D

Acq: 04 Dec 2019 14:52

Instrument :

MSVOA_D

ClientSampleId :


SB-6-(1-3)RE

Tot Ion: 98 Resp: 27762

Ion Ratio Lower Upper




98 100

100 67.2 52.6 79.0

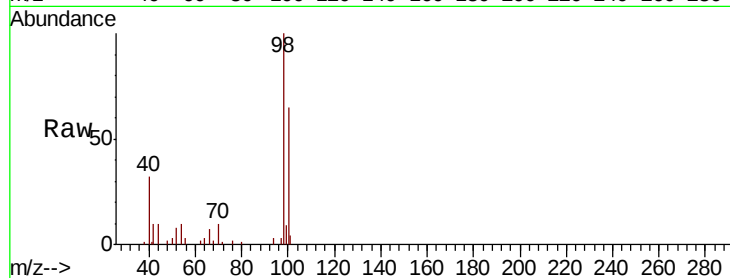

Abundance Ion 98.00 (97.70 to 98.70): VDC

Ion 100.00 (99.70 to 100.70): VDC

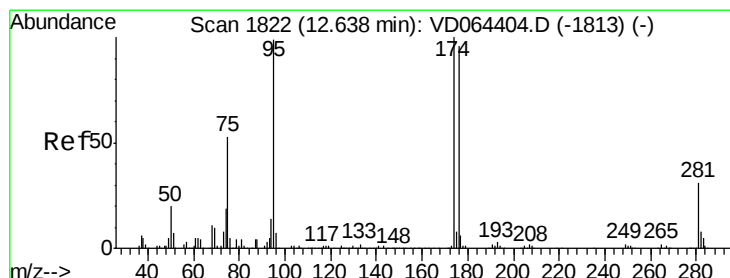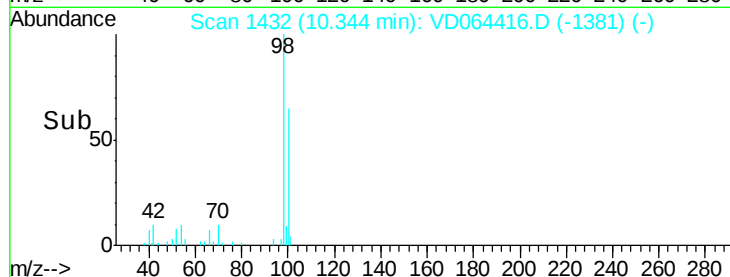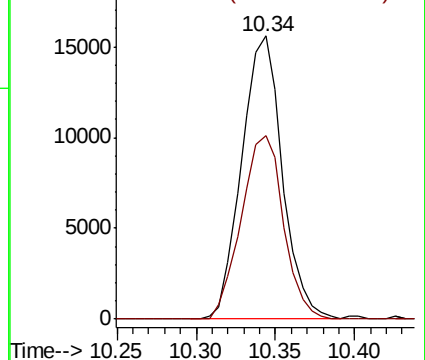

#62

4-Bromofluorobenzene

Concen: 56.683 ug/l

RT: 12.64 min Scan# 1822

Delta R.T. 0.00 min

Lab File: VD064416.D

Acq: 04 Dec 2019 14:52


Tgt Ion: 95 Resp: 10217

Ion Ratio Lower Upper

95 100

174 93.2 0.0 197.2



176 91.4 0.0 189.6

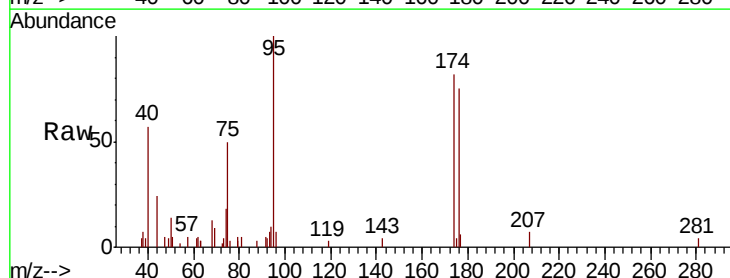


Abundance Ion 94.90 (94.60 to 95.60): VDC

Ion 173.80 (173.50 to 174.50): VDC

Ion 175.80 (175.50 to 176.50): VDC



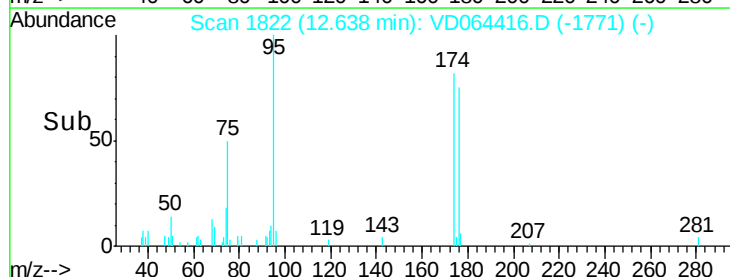
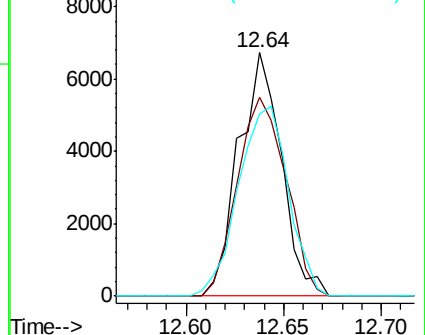


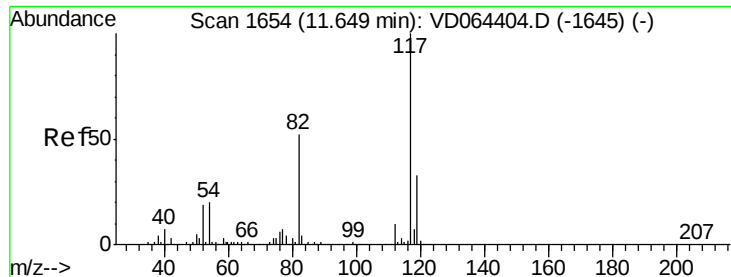

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.65 min Scan# 1654
Delta R.T. 0.00 min
Lab File: VD064416.D
Acq: 04 Dec 2019 14:52

Instrument :
MSVOA_D
ClientSampleId :
SB-6-(1-3)RE

Tot Ion	Ratio	Lower	Upper
117	100		
82	53.8	41.4	62.2
119	31.4	26.2	39.2

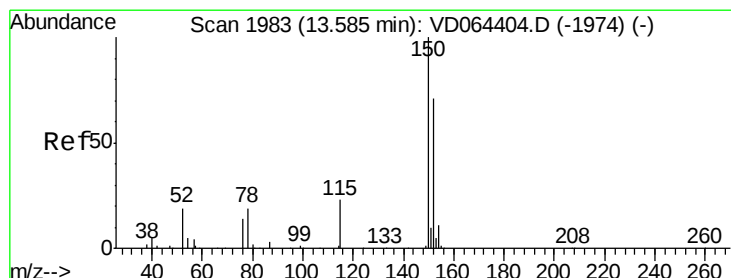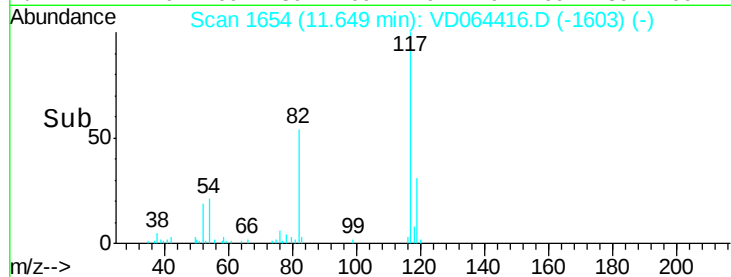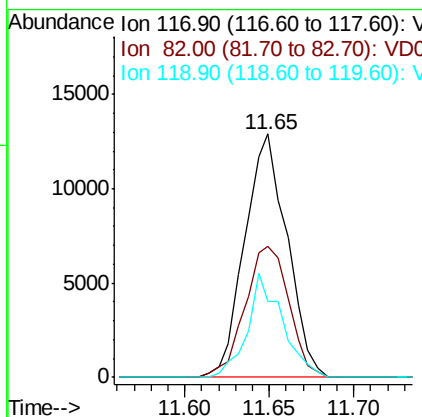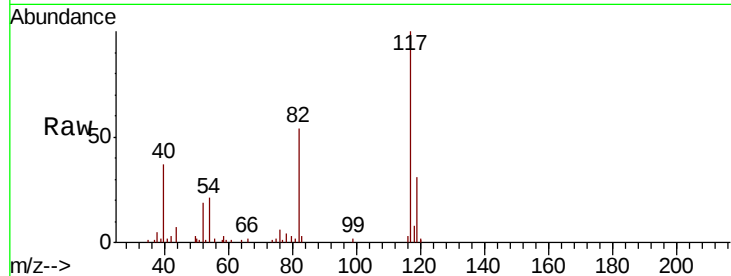

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.58 min Scan# 1983
Delta R.T. 0.00 min
Lab File: VD064416.D
Acq: 04 Dec 2019 14:52

Tgt Ion	Ratio	Lower	Upper
152	100		
115	59.1	26.7	80.1
150	150.6	0.0	347.2

