

Data Path : Z:\VOASRV\HPCHEM1\MSVOA D\DATA\VD120419\
 Data File : VD064421.D
 Acq On : 04 Dec 2019 17:16
 Operator : VA/SY
 Sample : K6119-12
 Misc : 4.14G/5.00ml/MSVOA D/SOIL
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_D
 ClientSampleId :
 SB-1-(8-10)

Quant Time: Dec 05 06:32:30 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_D\METHOD\82D112719S.M
 Quant Title : SW846 8260
 QLast Update : Fri Nov 29 07:18:03 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	7.98	168	641933	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	8.87	114	1050613	50.00	ug/l	0.00
63) Chlorobenzene-d5	11.65	117	946686	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.58	152	453347	50.00	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.34	65	277206	47.71	ug/l	0.00
Spiked Amount	50.000		Recovery	=	95.42%	
35) Dibromofluoromethane	7.92	113	318041	48.05	ug/l	0.00
Spiked Amount	50.000		Recovery	=	96.10%	
50) Toluene-d8	10.34	98	1248692	50.08	ug/l	0.00
Spiked Amount	50.000		Recovery	=	100.16%	
62) 4-Bromofluorobenzene	12.64	95	404420	50.47	ug/l	0.00
Spiked Amount	50.000		Recovery	=	100.94%	


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA D\DATA\VD120419\
Data File : VD064421.D
Acq On : 04 Dec 2019 17:16
Operator : VA/SY
Sample : K6119-12
Misc : 4.14G/5.00ml/MSVOA D/SOIL
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
SB-1-(8-10)

Quant Time: Dec 05 06:32:30 2019
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_D\METHOD\82D112719S.M
Quant Title : SW846 8260
QLast Update : Fri Nov 29 07:18:03 2019
Response via : Initial Calibration

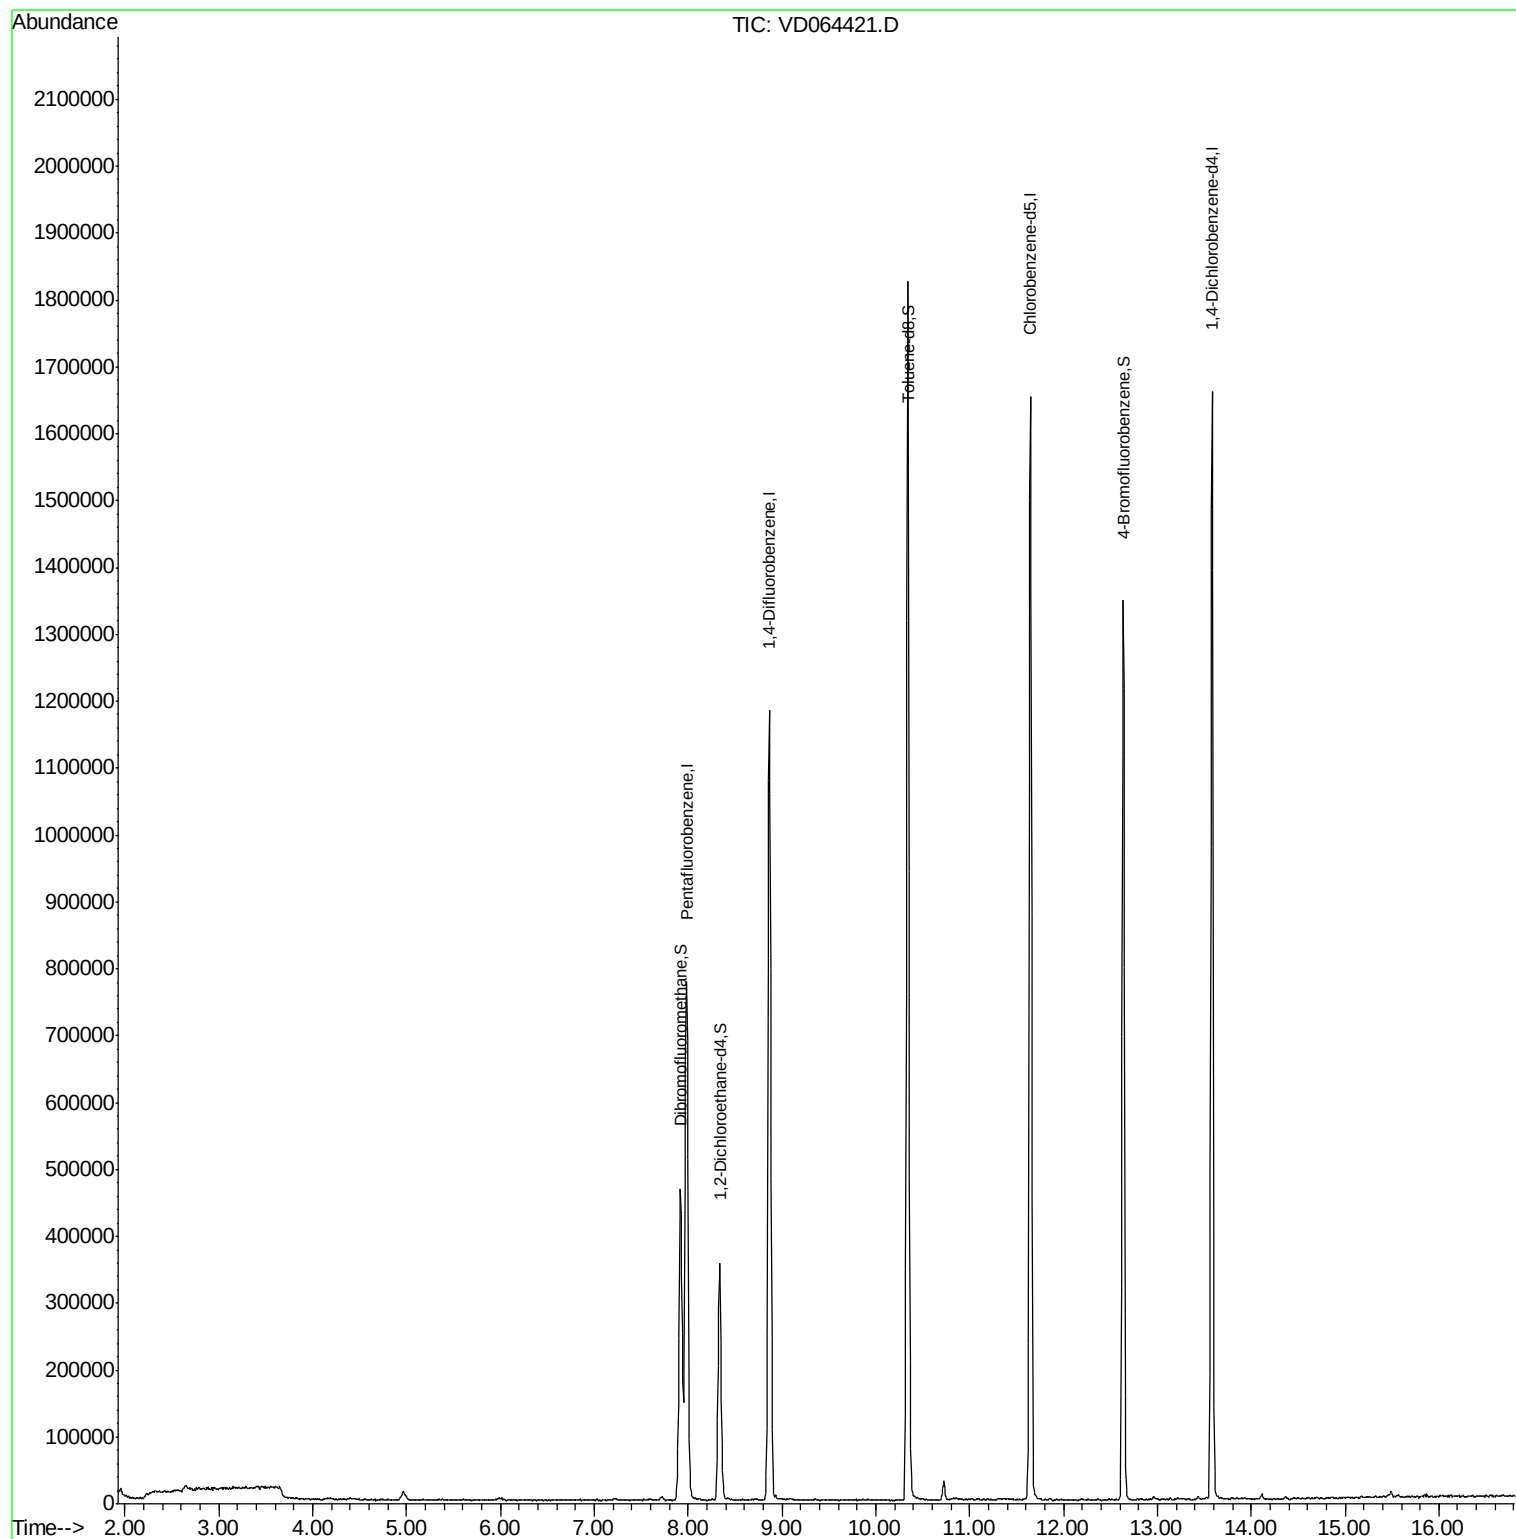

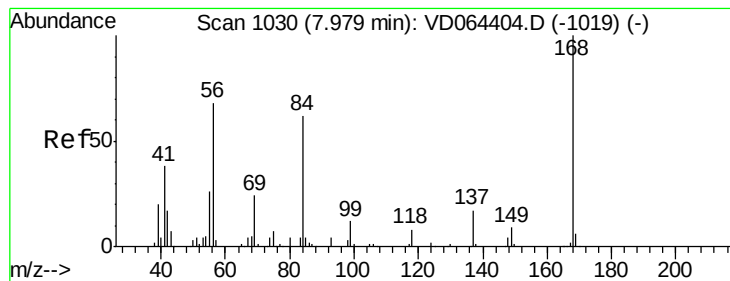

#1

Pentafluorobenzene

Concen: 50.000 ug/l

RT: 7.98 min Scan# 1031

Delta R.T. 0.01 min

Lab File: VD064421.D

Acq: 04 Dec 2019 17:16

Instrument :

MSVOA_D

ClientSampleId :


SB-1-(8-10)

Tot Ion:168 Resp: 641933

Ion Ratio Lower Upper




168 100

99 48.9 40.7 61.1

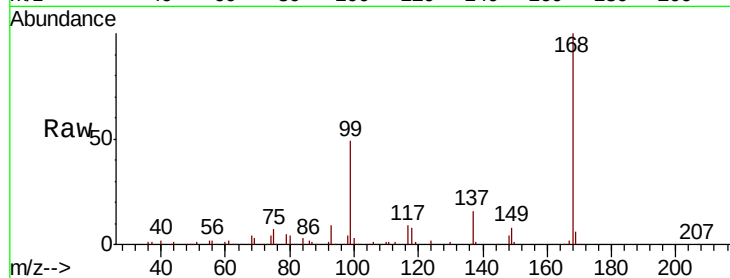

Abundance Ion 167.90 (167.60 to 168.60): V

Ion 98.90 (98.60 to 99.60): VDC

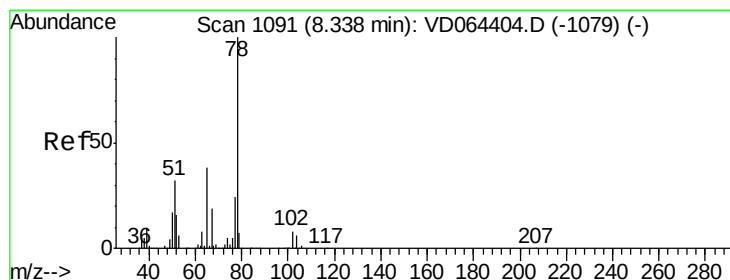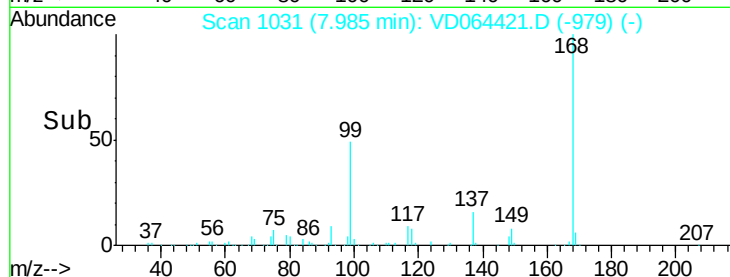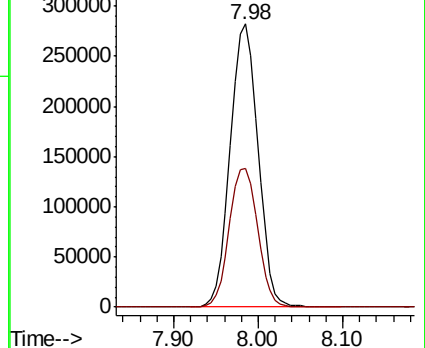

#33

1,2-Dichloroethane-d4

Concen: 47.708 ug/l

RT: 8.34 min Scan# 1091

Delta R.T. -0.00 min

Lab File: VD064421.D


Acq: 04 Dec 2019 17:16

Tgt Ion: 65 Resp: 277206

Ion Ratio Lower Upper



65 100


67 52.6 0.0 102.0

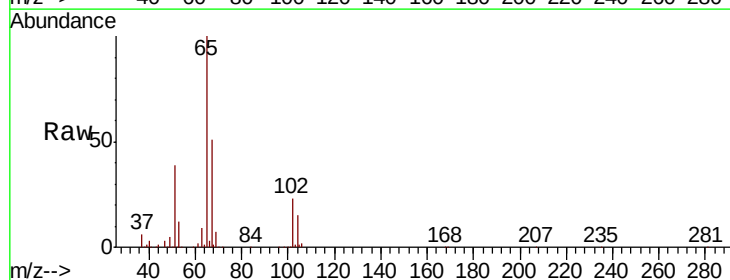

Abundance Ion 64.90 (64.60 to 65.60): VDC

Ion 66.90 (66.60 to 67.60): VDC

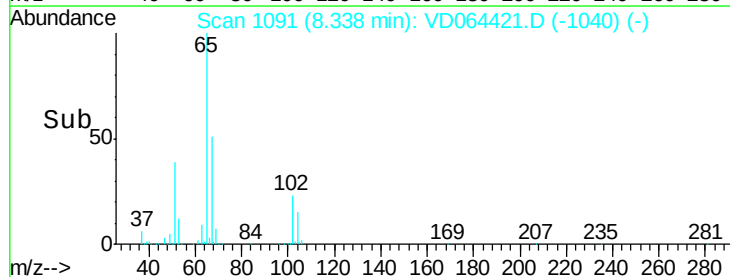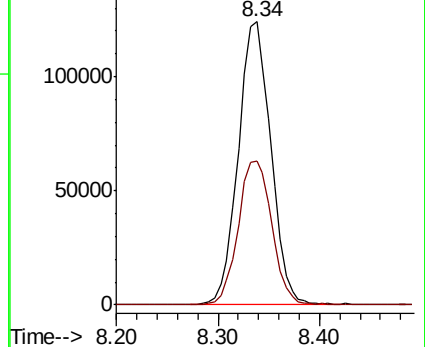


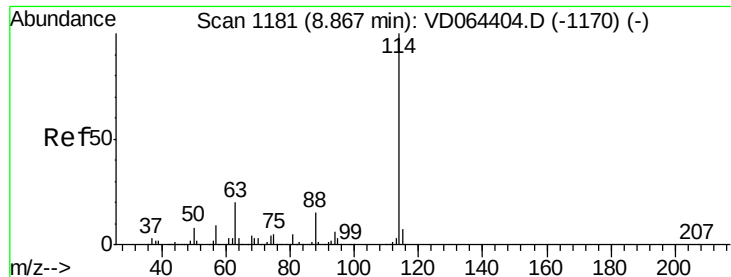




#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 8.87 min Scan# 1181
Delta R.T. -0.00 min
Lab File: VD064421.D
Acq: 04 Dec 2019 17:16

Instrument :
MSVOA_D
ClientSampleId :
SB-1-(8-10)

Tot Ion:114 Resp: 1050613
Ion Ratio Lower Upper
114 100
63 20.2 0.0 40.0
88 15.0 0.0 29.2

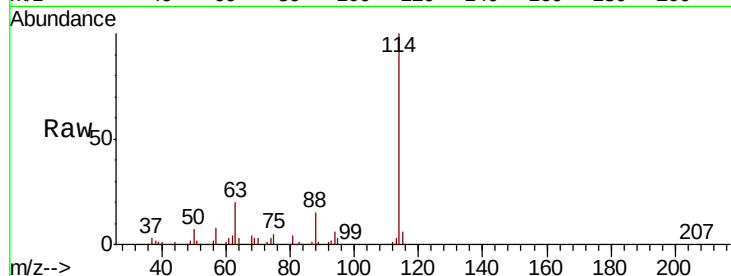


Abundance Ion 113.90 (113.60 to 114.60): V
Ion 63.00 (62.70 to 63.70): V
Ion 87.90 (87.60 to 88.60): V

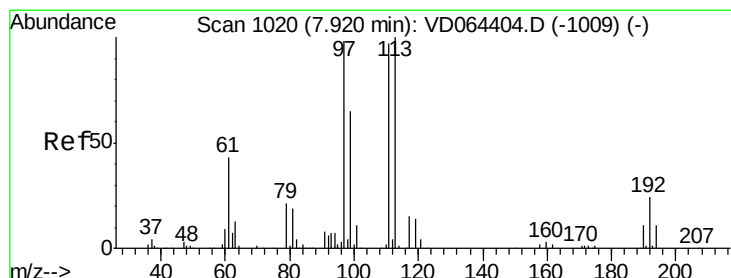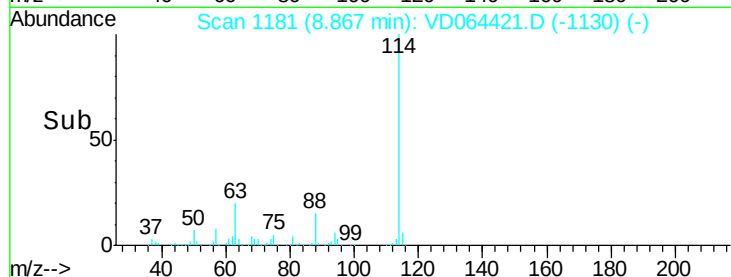
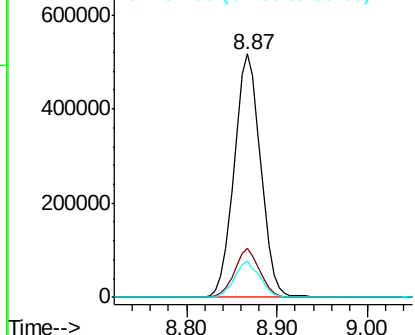



#35
Dibromofluoromethane
Concen: 48.047 ug/l
RT: 7.92 min Scan# 1020
Delta R.T. -0.00 min
Lab File: VD064421.D
Acq: 04 Dec 2019 17:16

Tgt Ion:113 Resp: 318041
Ion Ratio Lower Upper
113 100
111 101.6 79.4 119.2
192 23.1 18.6 28.0

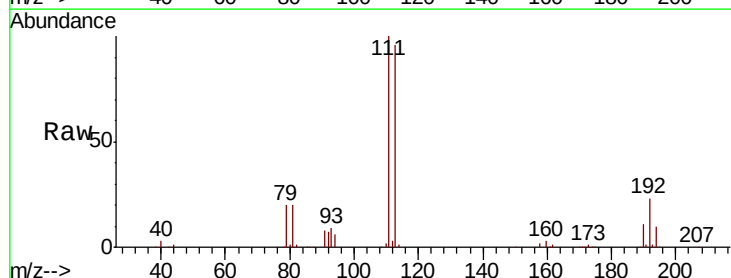

Abundance Ion 112.80 (112.50 to 113.50): V
Ion 110.80 (110.50 to 111.50): V
Ion 191.70 (191.40 to 192.40): V



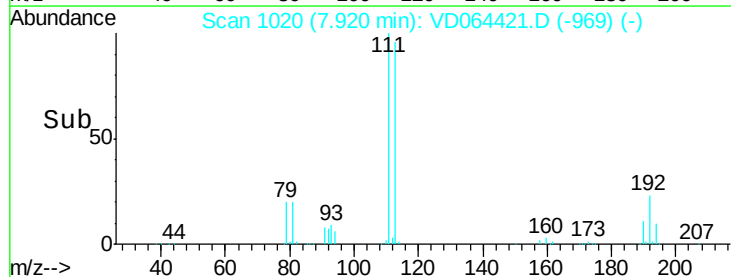
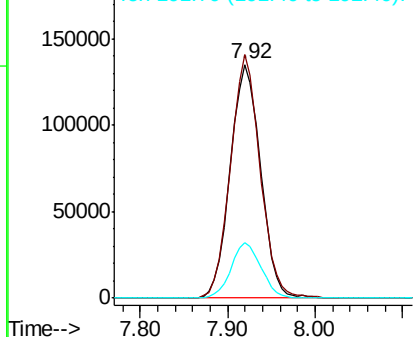


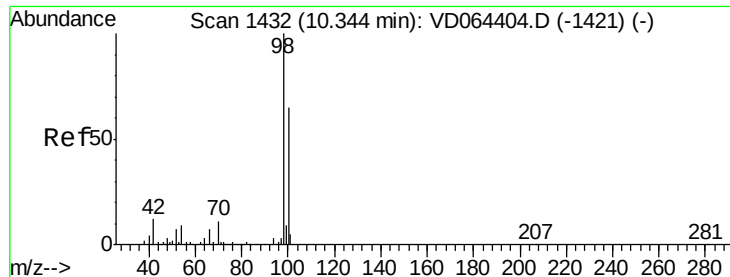

#50
Toluene-d8
Concen: 50.079 ug/l
RT: 10.34 min Scan# 1432
Delta R.T. -0.00 min
Lab File: VD064421.D
Acq: 04 Dec 2019 17:16




Instrument :
MSVOA_D
ClientSampleId :
SB-1-(8-10)


Tot Ion: 98 Resp: 1248692
Ion Ratio Lower Upper
98 100
100 66.1 52.6 79.0

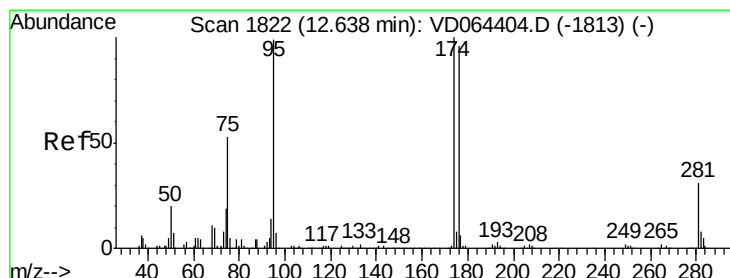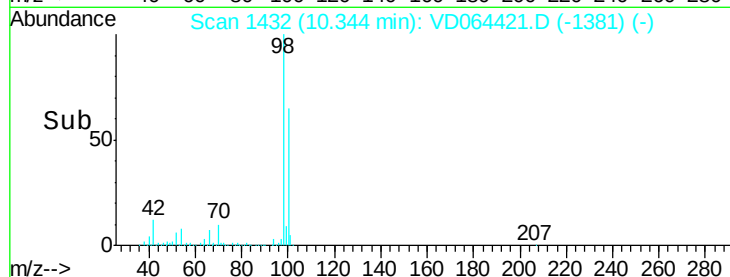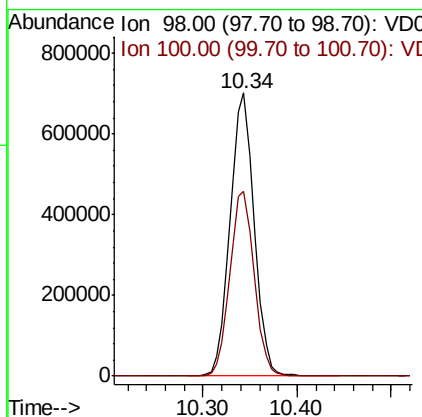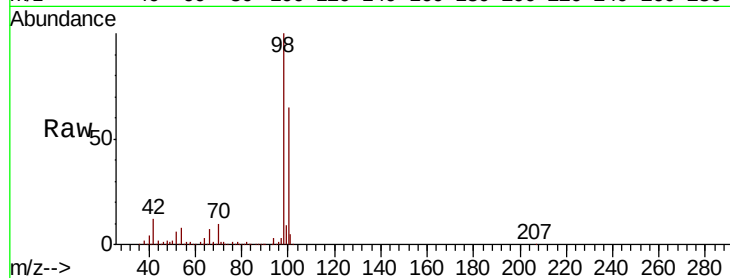

#62
4-Bromofluorobenzene
Concen: 50.469 ug/l
RT: 12.64 min Scan# 1822
Delta R.T. 0.00 min
Lab File: VD064421.D
Acq: 04 Dec 2019 17:16

Tgt Ion: 95 Resp: 404420
Ion Ratio Lower Upper
95 100
174 94.9 0.0 197.2
176 91.3 0.0 189.6


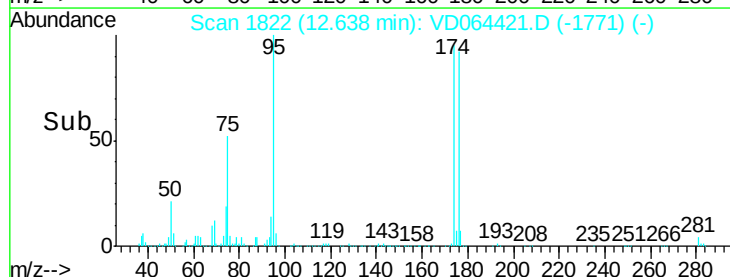
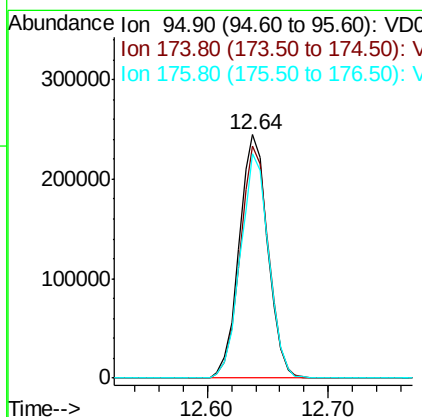
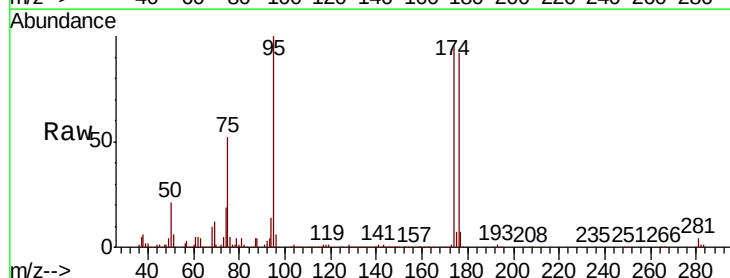


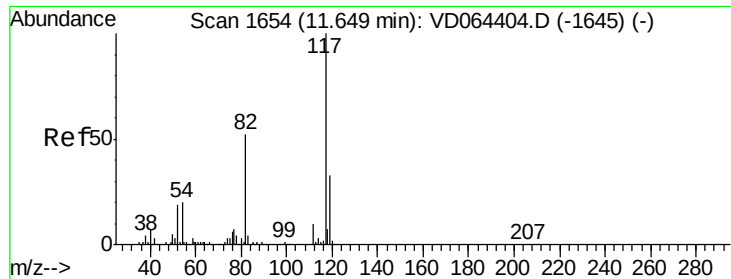

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.65 min Scan# 1654
Delta R.T. -0.00 min
Lab File: VD064421.D
Acq: 04 Dec 2019 17:16

Instrument :
MSVOA_D
ClientSampleId :
SB-1-(8-10)

Tot Ion:117 Resp: 946686
Ion Ratio Lower Upper
117 100
82 51.9 41.4 62.2
119 31.6 26.2 39.2

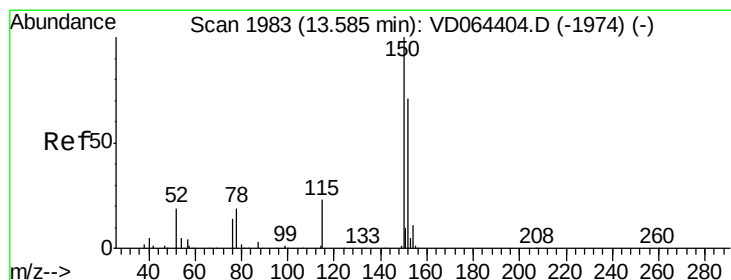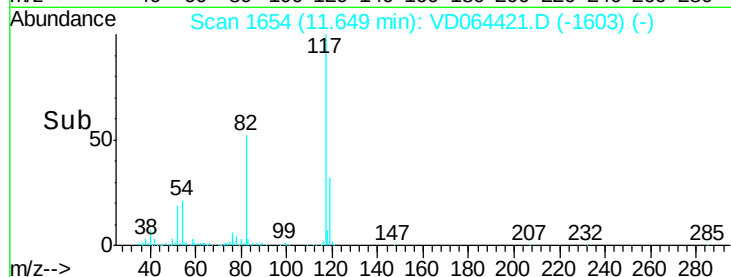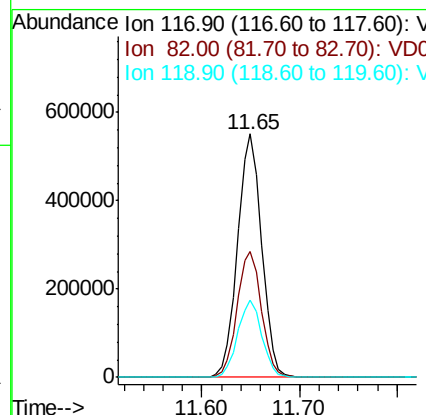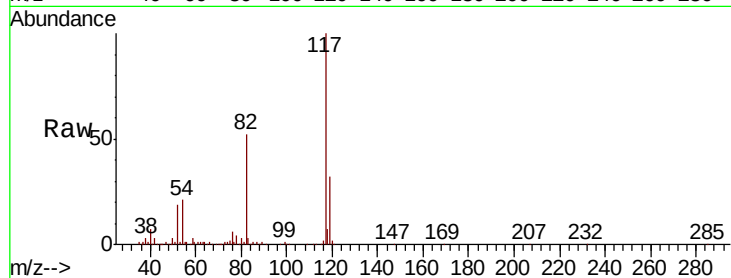

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.58 min Scan# 1983
Delta R.T. -0.00 min
Lab File: VD064421.D
Acq: 04 Dec 2019 17:16

Tgt Ion:152 Resp: 453347
Ion Ratio Lower Upper
152 100
115 53.6 26.7 80.1
150 156.0 0.0 347.2

