


Data Path : Z:\voasrv\HPCHEM1\MSVOA D\Data\VD120919\
Data File : VD064468.D
Acq On : 09 Dec 2019 10:00
Operator : VA/SY
Sample : BFB
Misc : 5.00G/5.00ml/MSVOA D/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_D\METHOD\82D112719S.M
Title : SW846 8260
Last Update : Fri Nov 29 07:18:03 2019

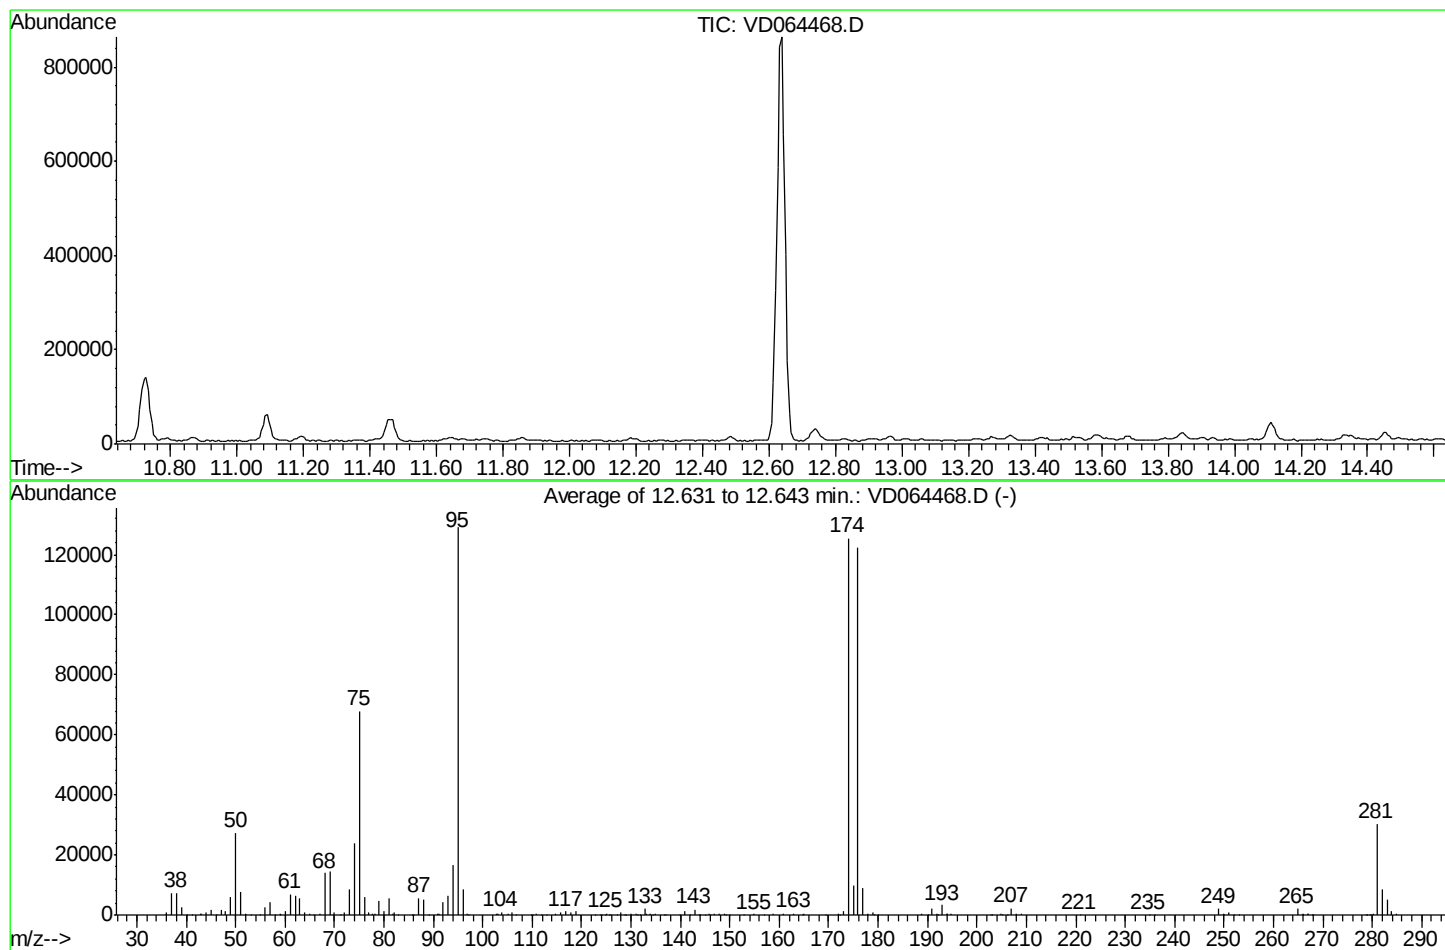

AutoFind: Scans 1821, 1822, 1823; Background Corrected with Scan 1811

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	21.2	27402	PASS
75	95	30	60	52.6	67861	PASS
95	95	100	100	100.0	129106	PASS
96	95	5	9	6.5	8431	PASS
173	174	0.00	2	1.0	1225	PASS
174	95	50	100	97.2	125434	PASS
175	174	5	9	7.8	9725	PASS
176	174	95	101	97.5	122346	PASS
177	176	5	9	7.3	8977	PASS