


Data Path : Z:\voasrv\HPCHEM1\MSVOA D\Data\VD120920\
Data File : VD067916.D
Acq On : 09 Dec 2020 09:17
Operator : VA/SY
Sample : BFB
Misc : 5.00G/5.00ml/MSVOA D/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_D\METHOD\82D120120S.M
Title : SW846 8260
Last Update : Wed Dec 02 08:05:58 2020

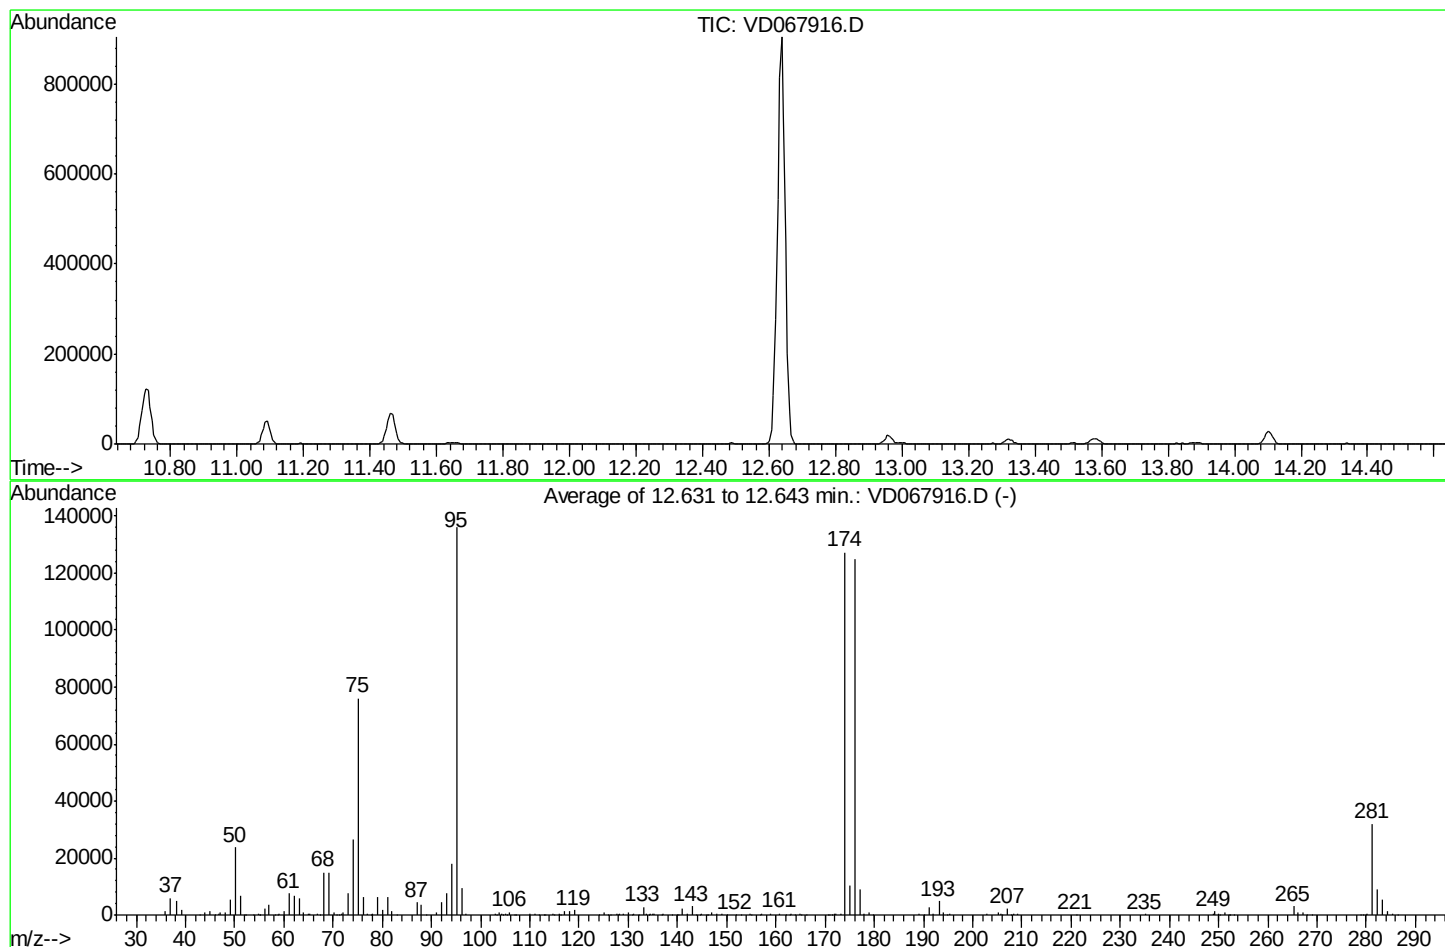

AutoFind: Scans 1821, 1822, 1823; Background Corrected with Scan 1812

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.5	23778	PASS
75	95	30	60	55.8	75986	PASS
95	95	100	100	100.0	136098	PASS
96	95	5	9	6.9	9327	PASS
173	174	0.00	2	0.5	617	PASS
174	95	50	100	93.6	127376	PASS
175	174	5	9	8.2	10397	PASS
176	174	95	101	97.9	124733	PASS
177	176	5	9	7.4	9191	PASS