
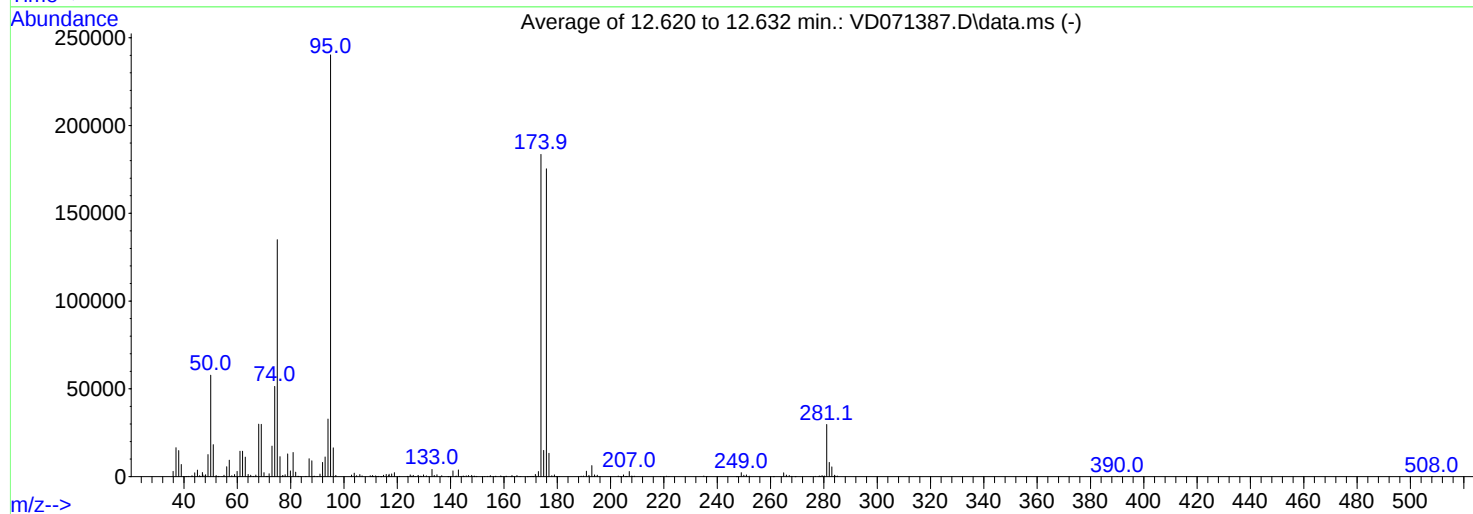


Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD122021\
 Data File : VD071387.D
 Acq On : 20 Dec 2021 11:36
 Operator : VA/SY
 Sample : BFB
 Misc : 5.00G/5.00ml/MSVOA_D/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_D
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D112921S.M
 Title : SW846 8260
 Last Update : Mon Nov 29 17:54:09 2021

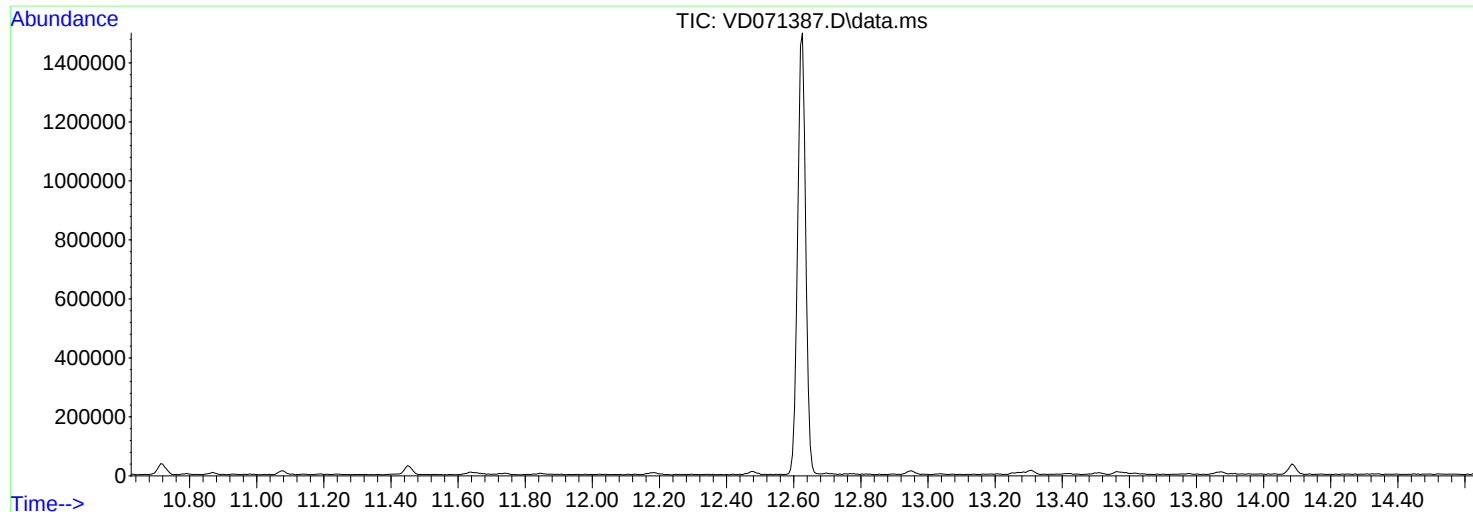

AutoFind: Scans 1819, 1820, 1821; Background Corrected with Scan 1809

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	24.1	57797	PASS
75	95	30	60	56.2	134989	PASS
95	95	100	100	100.0	240256	PASS
96	95	5	9	6.8	16440	PASS
173	174	0.00	2	1.6	2885	PASS
174	95	50	100	76.4	183595	PASS
175	174	5	9	8.1	14961	PASS
176	174	95	101	95.5	175339	PASS
177	176	5	9	7.6	13333	PASS