


Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD122820\
Data File : VD067951.D
Acq On : 28 Dec 2020 09:27
Operator : VA/SY
Sample : BFB
Misc : 5.00G/5.00ml/MSVOA_D/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D122220S.M
Title : Sw846 8260
Last Update : Wed Dec 23 07:34:16 2020

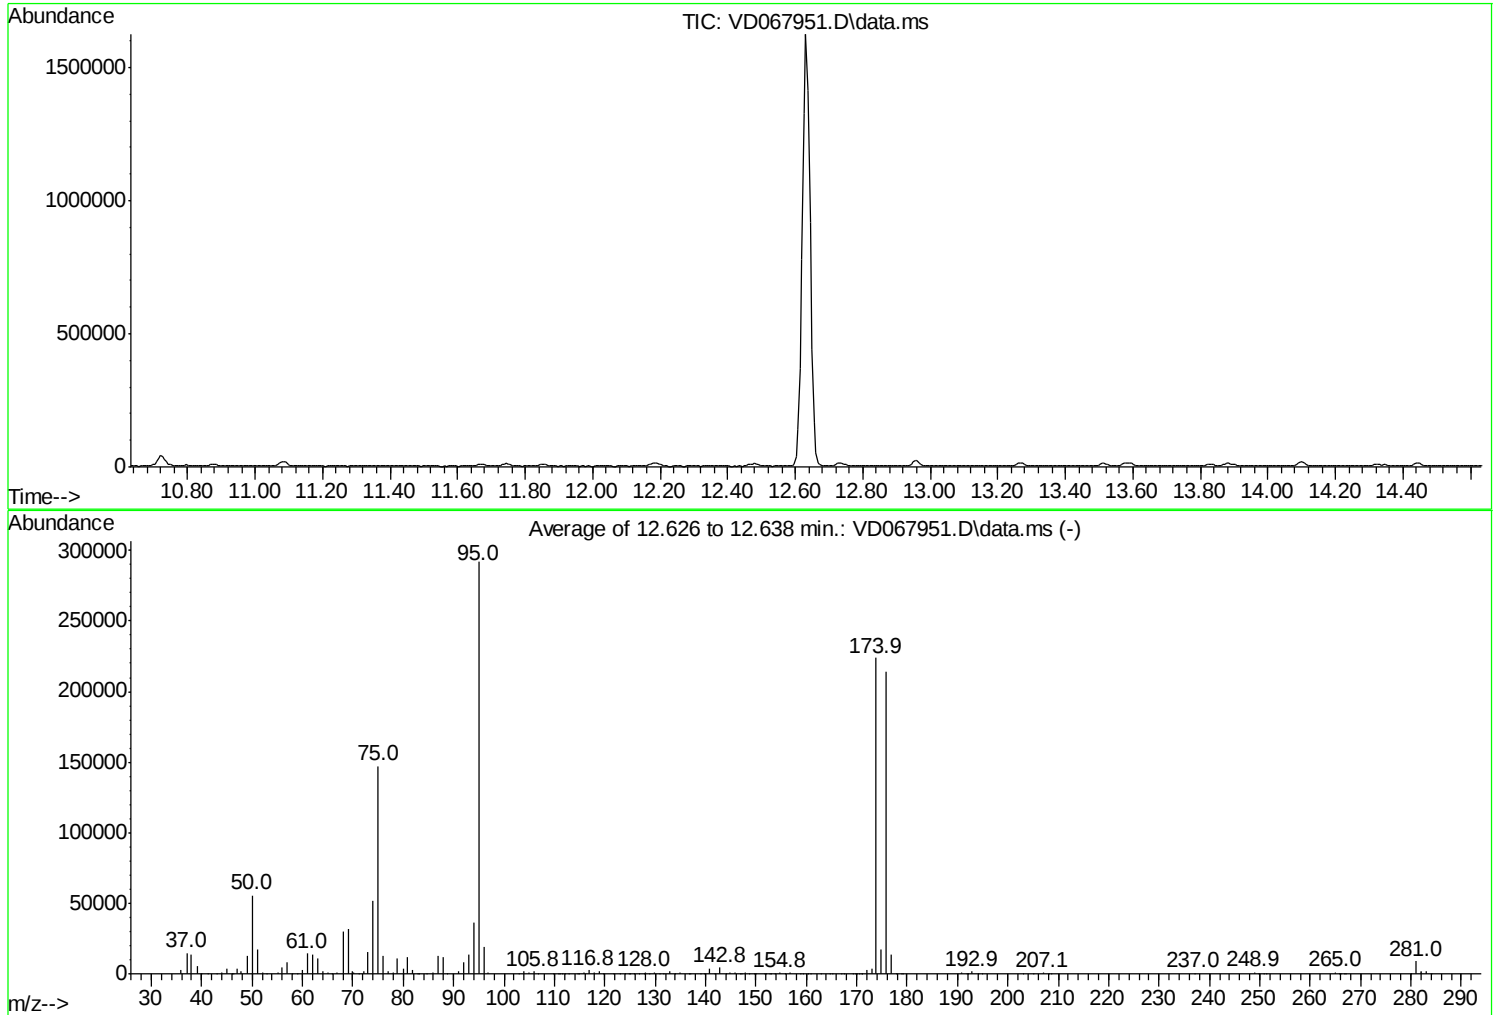

AutoFind: Scans 1820, 1821, 1822; Background Corrected with Scan 1810

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	19.0	55440	PASS
75	95	30	60	50.3	146965	PASS
95	95	100	100	100.0	291989	PASS
96	95	5	9	6.5	18952	PASS
173	174	0.00	2	1.7	3795	PASS
174	95	50	100	76.7	223979	PASS
175	174	5	9	7.8	17499	PASS
176	174	95	101	95.7	214443	PASS
177	176	5	9	6.5	13840	PASS