


Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD122920\
Data File : VD067960.D
Acq On : 29 Dec 2020 09:32
Operator : VA/SY
Sample : BFB
Misc : 5.00G/5.00ml/MSVOA_D/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D122220S.M
Title : Sw846 8260
Last Update : Wed Dec 23 07:34:16 2020

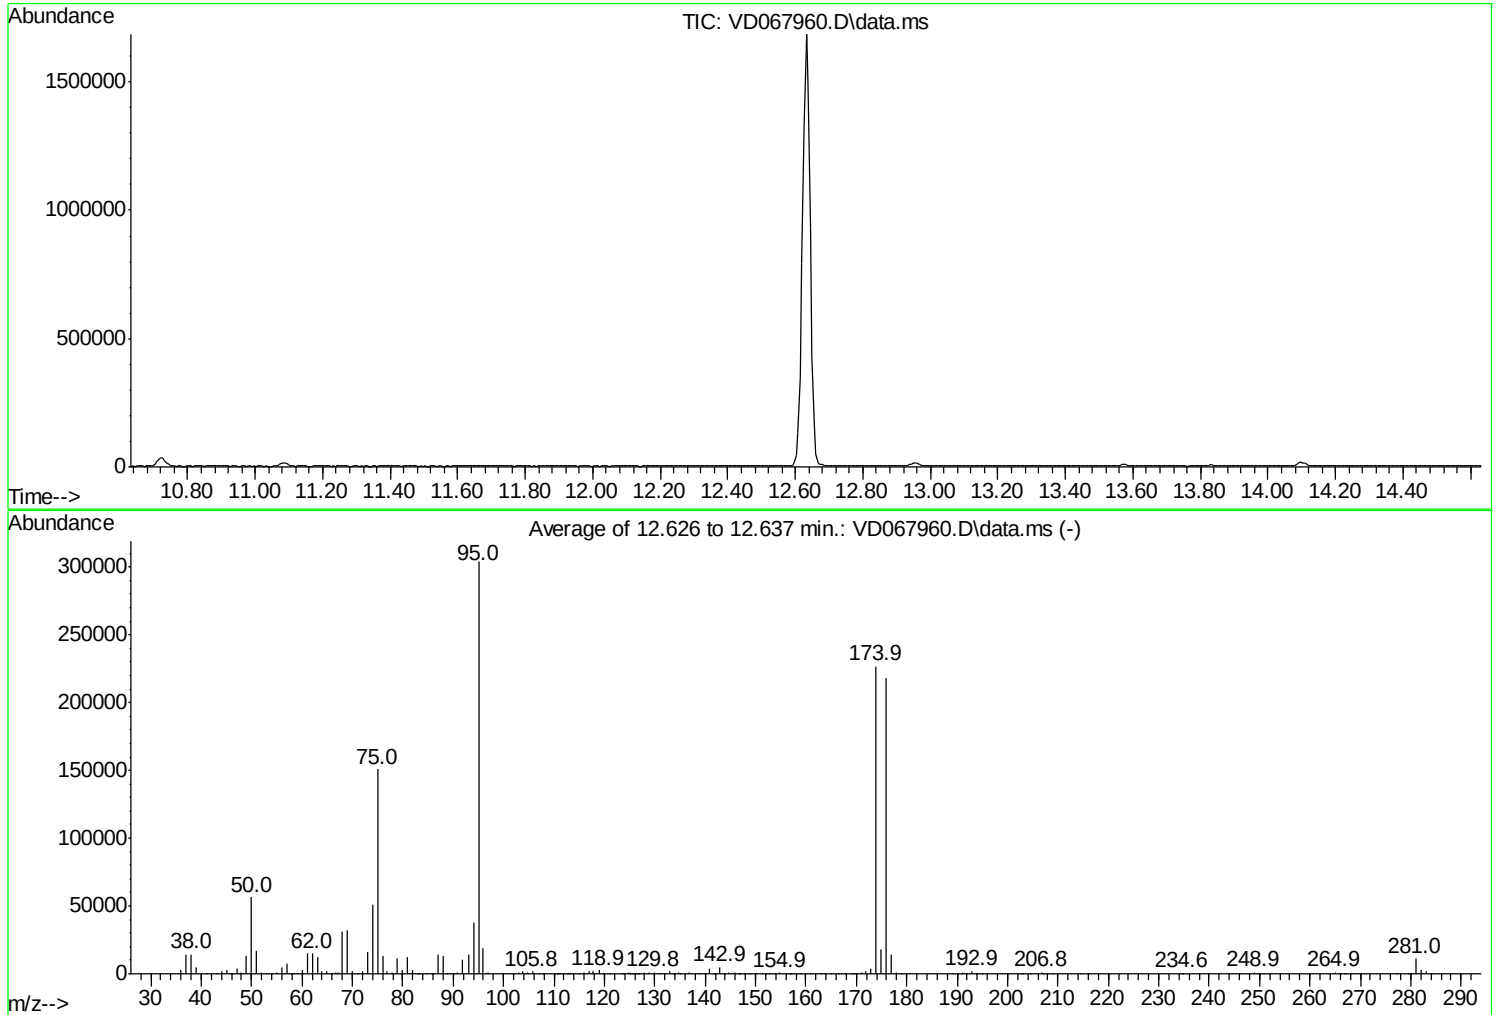

AutoFind: Scans 1820, 1821, 1822; Background Corrected with Scan 1810

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.6	56557	PASS
75	95	30	60	49.6	150699	PASS
95	95	100	100	100.0	303851	PASS
96	95	5	9	6.2	18891	PASS
173	174	0.00	2	1.8	4171	PASS
174	95	50	100	74.6	226752	PASS
175	174	5	9	7.8	17783	PASS
176	174	95	101	96.2	218240	PASS
177	176	5	9	6.5	14206	PASS