
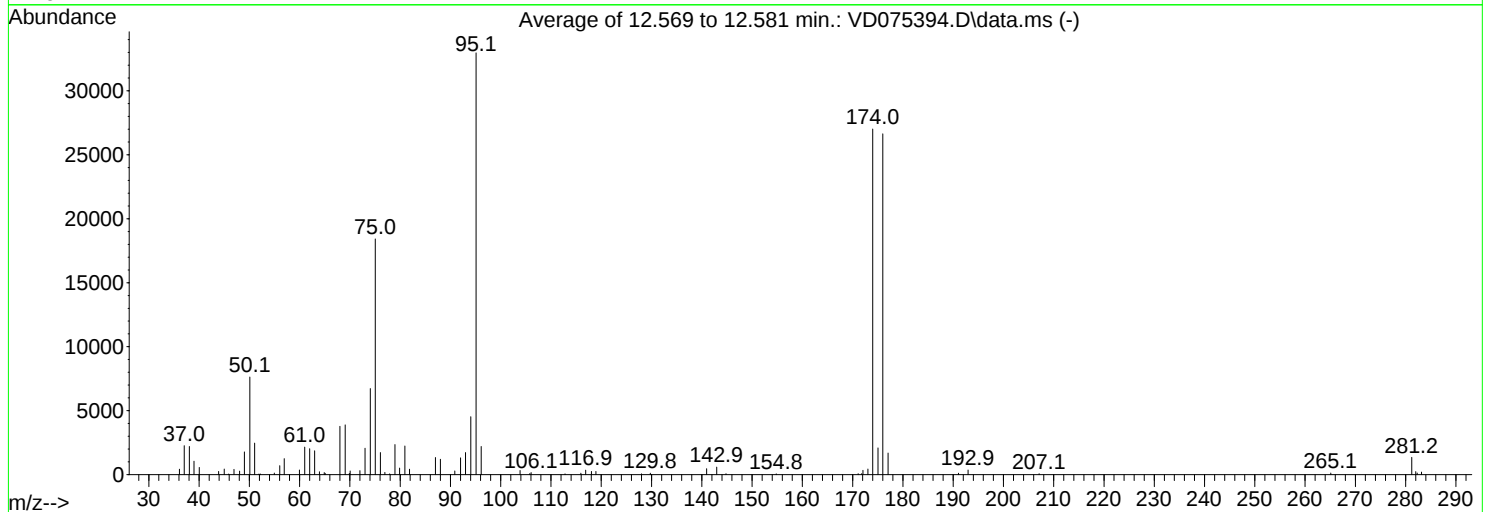


Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD022223\
Data File : VD075394.D
Acq On : 22 Feb 2023 10:32
Operator : KP/SY
Sample : BFB
Misc : 5.00G/5.00ml/MSVOA_D/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D022123S.M
Title : SW846 8260
Last Update : Tue Feb 21 16:26:04 2023

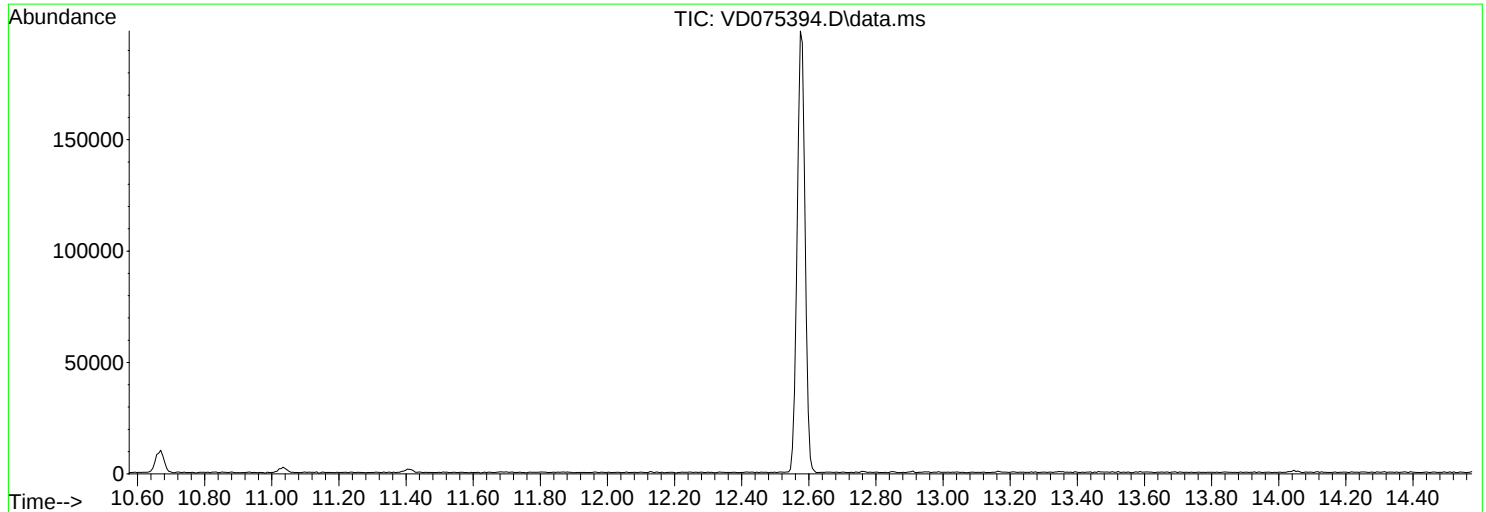

AutoFind: Scans 1867, 1868, 1869; Background Corrected with Scan 1860

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	23.1	7625	PASS
75	95	30	60	55.9	18425	PASS
95	95	100	100	100.0	32968	PASS
96	95	5	9	6.7	2196	PASS
173	174	0.00	2	1.6	432	PASS
174	95	50	100	82.0	27019	PASS
175	174	5	9	7.7	2092	PASS
176	174	95	101	98.6	26635	PASS
177	176	5	9	6.4	1695	PASS