
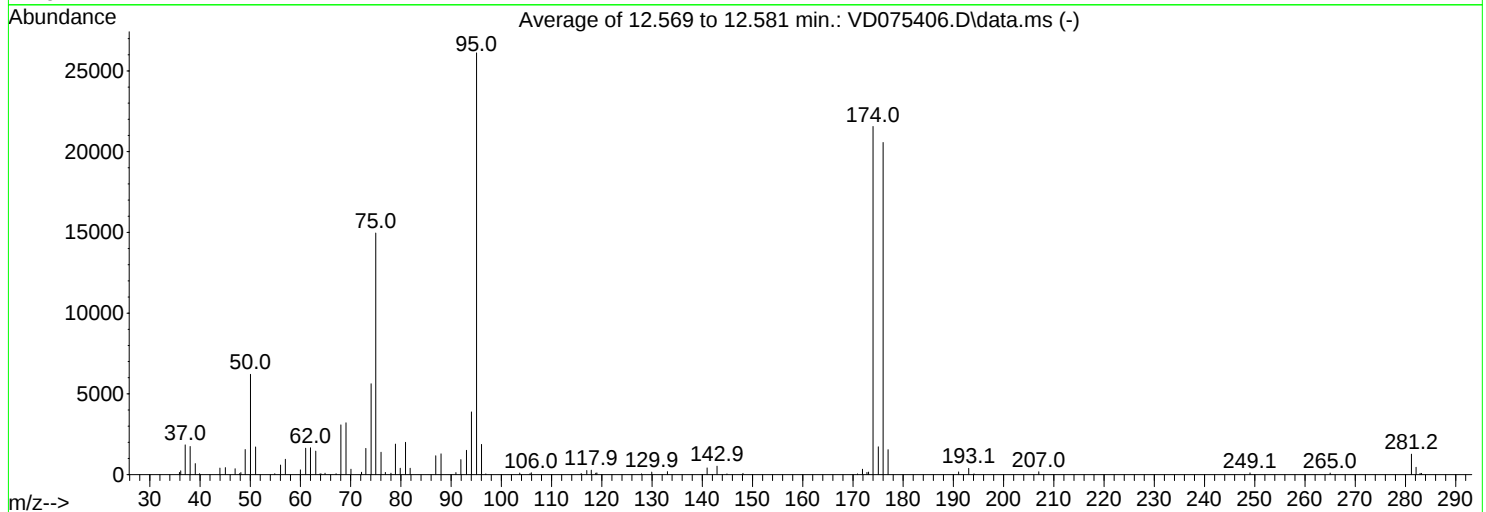


Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD022323\
Data File : VD075406.D
Acq On : 23 Feb 2023 09:50
Operator : KP/SY
Sample : BFB101
Misc : 5.00G/5.00ml/MSVOA_D/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
BFB101

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\SFAMDLM022323SMA.M
Title : SFAM01.0
Last Update : Thu Feb 23 23:55:37 2023

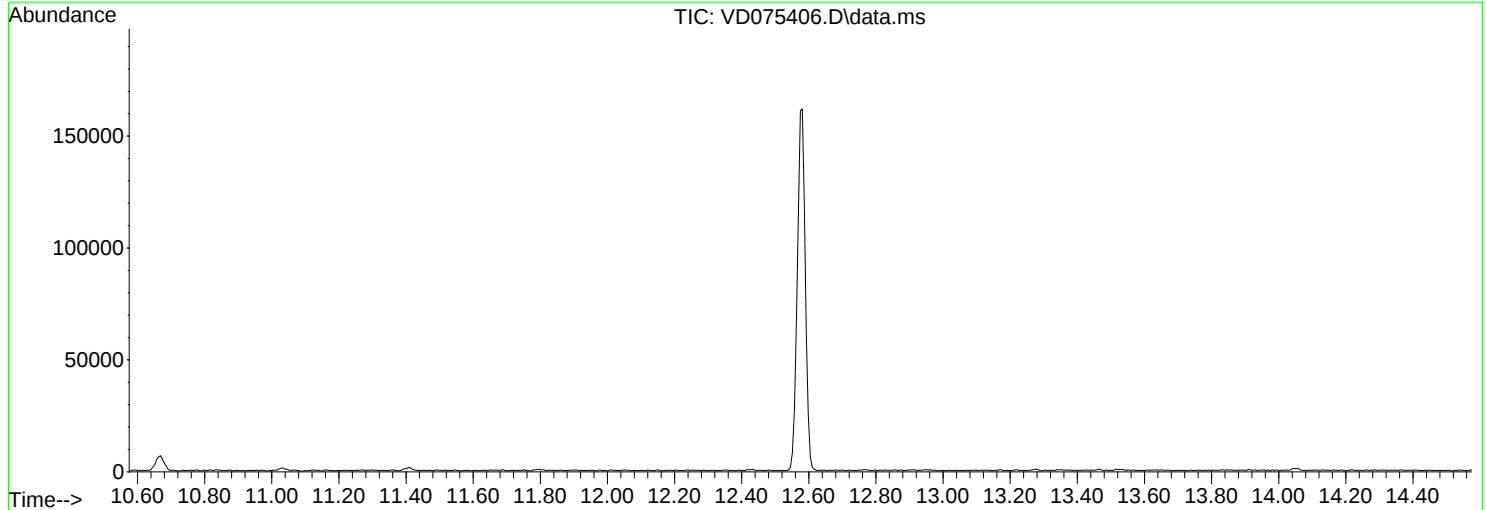

AutoFind: Scans 1867, 1868, 1869; Background Corrected with Scan 1860

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	23.8	6215	PASS
75	95	30	80	57.3	14965	PASS
95	95	100	100	100.0	26117	PASS
96	95	5	9	7.2	1872	PASS
173	174	0.00	2	0.7	159	PASS
174	95	50	120	82.6	21560	PASS
175	174	5	9	8.0	1728	PASS
176	174	95	105	95.4	20571	PASS
177	176	5	10	7.5	1542	PASS

Scan 1860 (12.528 min): VD075406.D\data.ms
BFB101

m/z	Abundance
39.90	428.0
44.00	168.0

Instrument :
MSVOA_D
ClientSampleId :
BFB101

m/z	Abundance
36.30	256.0
37.00	1771.0
38.00	1564.0
39.10	619.0
40.00	569.0
43.90	569.0
45.10	396.0
47.00	258.0
48.20	185.0
49.00	1299.0
50.10	5716.0
51.00	1306.0
56.00	615.0
57.20	657.0
60.00	299.0
61.00	1500.0
62.00	1177.0
63.00	1226.0
63.90	160.0
64.10	158.0
68.10	2218.0
69.10	2619.0
70.10	211.0
73.00	1228.0
74.10	4290.0
75.00	12275.0
76.00	1141.0
76.90	168.0
78.90	1464.0
79.80	297.0
80.90	1830.0
81.80	203.0
87.00	896.0
88.00	1096.0
91.90	706.0
93.10	1309.0
94.10	3467.0
95.00	21080.0
96.10	1426.0
117.10	266.0
117.80	220.0
129.90	205.0
141.00	381.0
143.00	443.0
170.90	157.0
171.90	293.0
173.10	476.0
174.00	17032.0
175.00	1382.0
176.00	15617.0
177.00	1384.0
193.00	203.0
281.20	525.0
282.10	269.0

Instrument :
MSVOA_D
ClientSampleId :
BFB101

m/z	Abundance
36.10	445.0
37.10	1826.0
38.10	1730.0
39.00	831.0
39.90	353.0
44.00	562.0
45.00	428.0
47.00	394.0
47.90	210.0
49.00	1792.0
50.00	6741.0
51.10	1943.0
54.90	170.0
56.10	624.0
57.00	1288.0
60.10	225.0
61.10	1729.0
62.00	1905.0
63.00	1706.0
64.90	261.0
68.00	3588.0
69.10	3667.0
69.90	243.0
70.20	255.0
72.10	252.0
73.00	1848.0
74.00	6307.0
75.00	16379.0
76.00	1696.0
78.90	2201.0
79.90	432.0
80.90	2306.0
81.90	580.0
87.00	1312.0
88.00	1471.0
90.90	200.0
92.00	1149.0
93.10	1603.0
94.10	4241.0
95.10	28912.0
96.00	2193.0
103.70	154.0
105.70	177.0
106.00	181.0
115.90	208.0
116.90	304.0
117.90	159.0
118.80	267.0
127.90	153.0
133.00	231.0
140.90	473.0
143.00	554.0
171.80	339.0
174.00	23560.0
175.10	1835.0
176.00	22440.0
177.00	1441.0
191.10	204.0
193.00	448.0
207.10	276.0
249.00	174.0
281.20	1168.0
282.00	485.0

Instrument :
MSVOA_D
ClientSampleId :
BFB101

m/z	Abundance
35.90	404.0
37.10	1924.0
38.00	1928.0
39.00	601.0
39.90	532.0
44.00	581.0
45.10	475.0
47.00	452.0
48.10	215.0
49.00	1567.0
50.10	6187.0
51.00	1901.0
56.00	538.0
56.90	898.0
59.90	369.0
61.00	1688.0
62.00	1912.0
63.10	1428.0
67.10	165.0
68.00	3440.0
69.00	3355.0
70.10	304.0
72.20	186.0
73.00	1814.0
74.00	6283.0
75.00	16241.0
76.10	1312.0
76.90	243.0
78.00	281.0
78.90	1999.0
79.90	458.0
80.90	1871.0
81.90	421.0
86.90	1288.0
88.00	1313.0
91.00	190.0
92.00	951.0
93.00	1600.0
94.00	3934.0
95.10	28360.0
96.10	1998.0
96.90	154.0
103.60	156.0
105.90	179.0
117.00	204.0
117.90	440.0
119.00	322.0
130.00	265.0
133.10	334.0
141.00	408.0
142.90	569.0
144.90	152.0
148.10	226.0
172.00	374.0
172.80	409.0
174.00	24088.0
175.00	1968.0
176.00	23656.0
177.00	1800.0
191.00	287.0
193.10	514.0
194.10	156.0
206.90	250.0
249.10	167.0
265.00	301.0
281.20	2101.0
282.20	607.0
282.90	224.0
283.20	231.0

Instrument :
MSVOA_D
ClientSampleId :
BFB101