
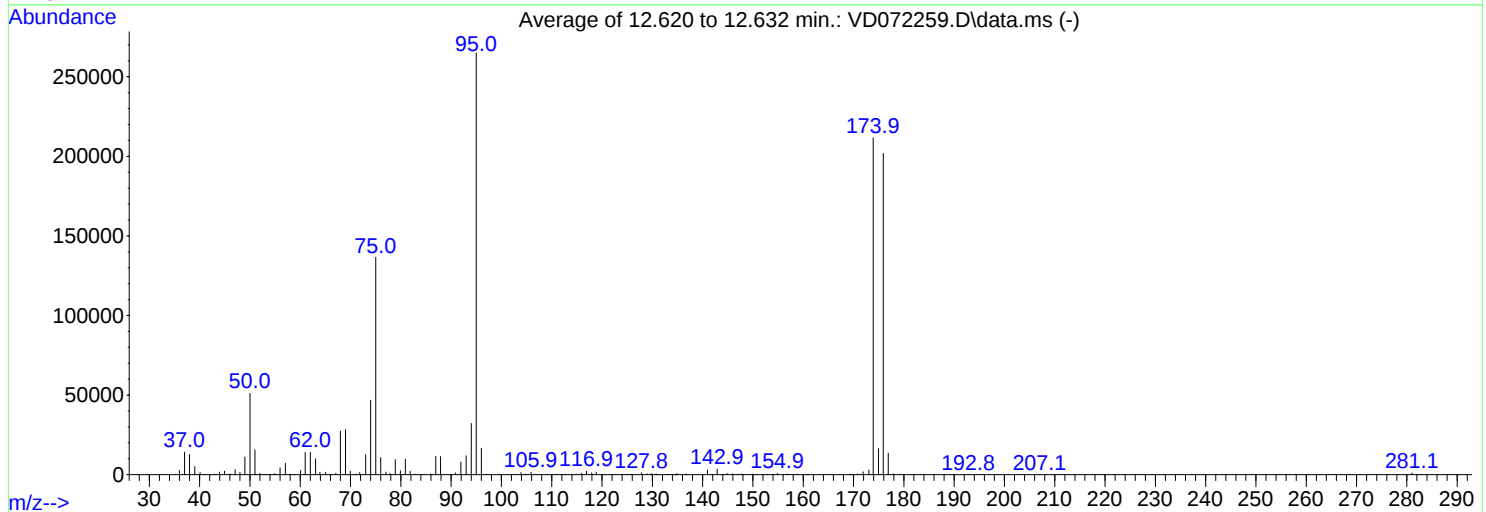


Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD031722\
 Data File : VD072259.D
 Acq On : 17 Mar 2022 23:10
 Operator : VA/SY
 Sample : BFB
 Misc : 5.00G/5.00ml/MSVOA_D/SOIL
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 MSVOA_D
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D031122S.M
 Title : SW846 8260
 Last Update : Mon Mar 14 05:18:06 2022

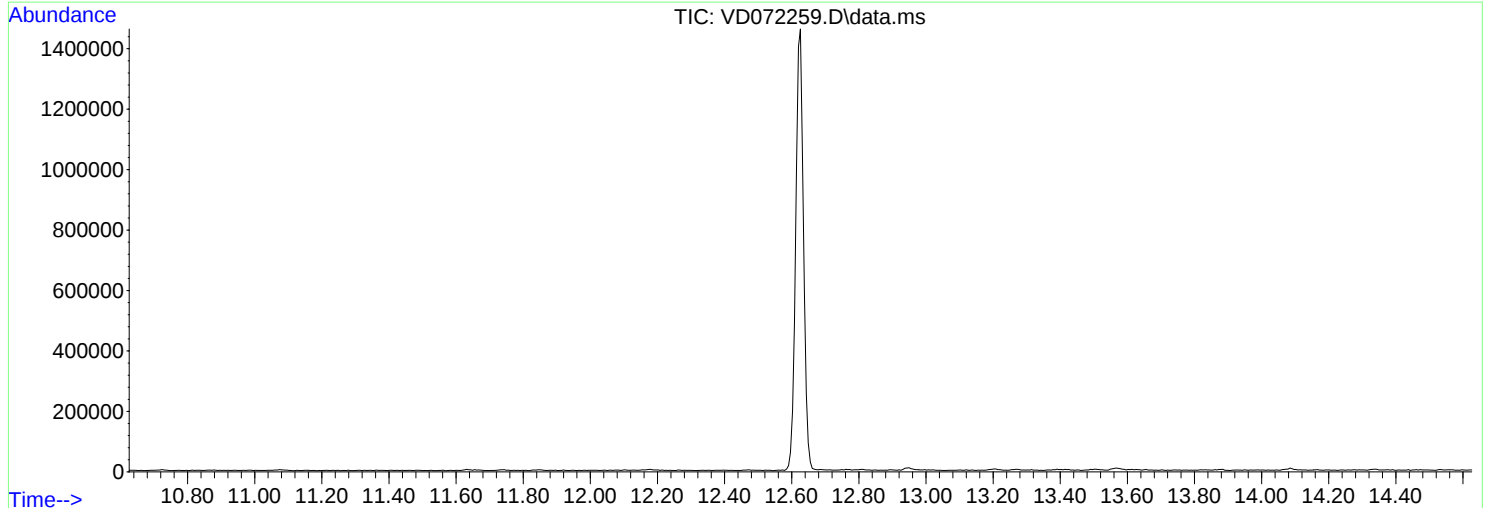

AutoFind: Scans 1819, 1820, 1821; Background Corrected with Scan 1810

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.3	51112	PASS
75	95	30	60	51.5	136515	PASS
95	95	100	100	100.0	265045	PASS
96	95	5	9	6.3	16610	PASS
173	174	0.00	2	1.4	2916	PASS
174	95	50	100	79.9	211691	PASS
175	174	5	9	7.8	16442	PASS
176	174	95	101	95.4	201899	PASS
177	176	5	9	6.7	13518	PASS