
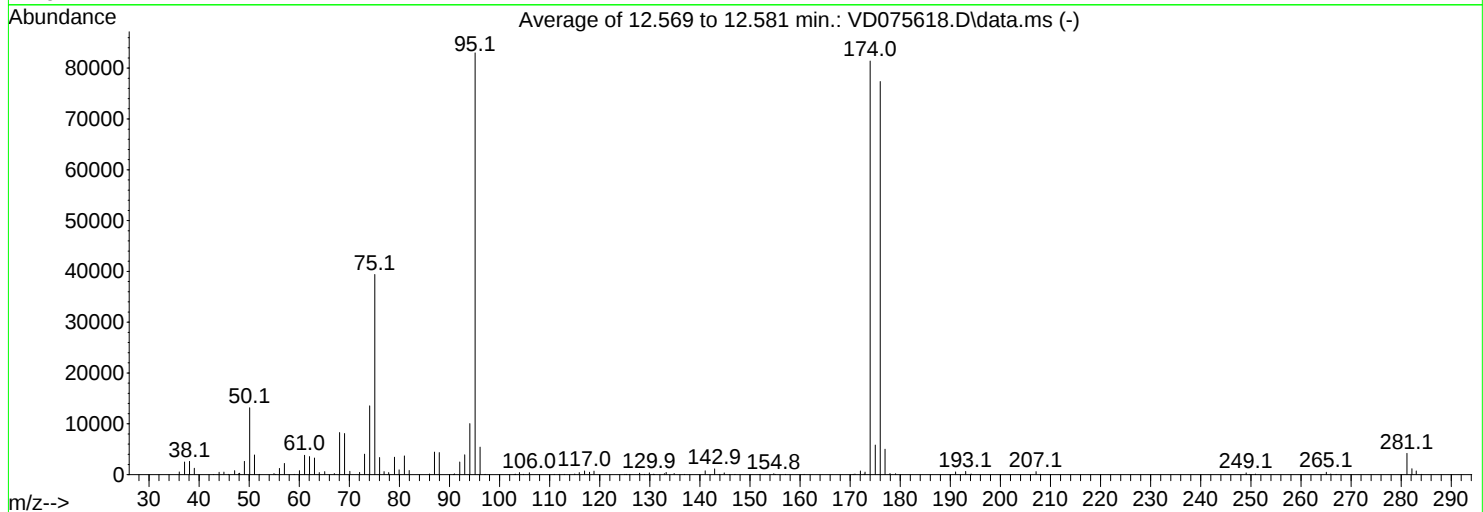


Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD041123\
Data File : VD075618.D
Acq On : 11 Apr 2023 09:08
Operator : KP/SY
Sample : BFB
Misc : 5.00G/5.00ml/MSVOA_D/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D041023S.M
Title : SW846 8260
Last Update : Wed Apr 12 10:29:09 2023

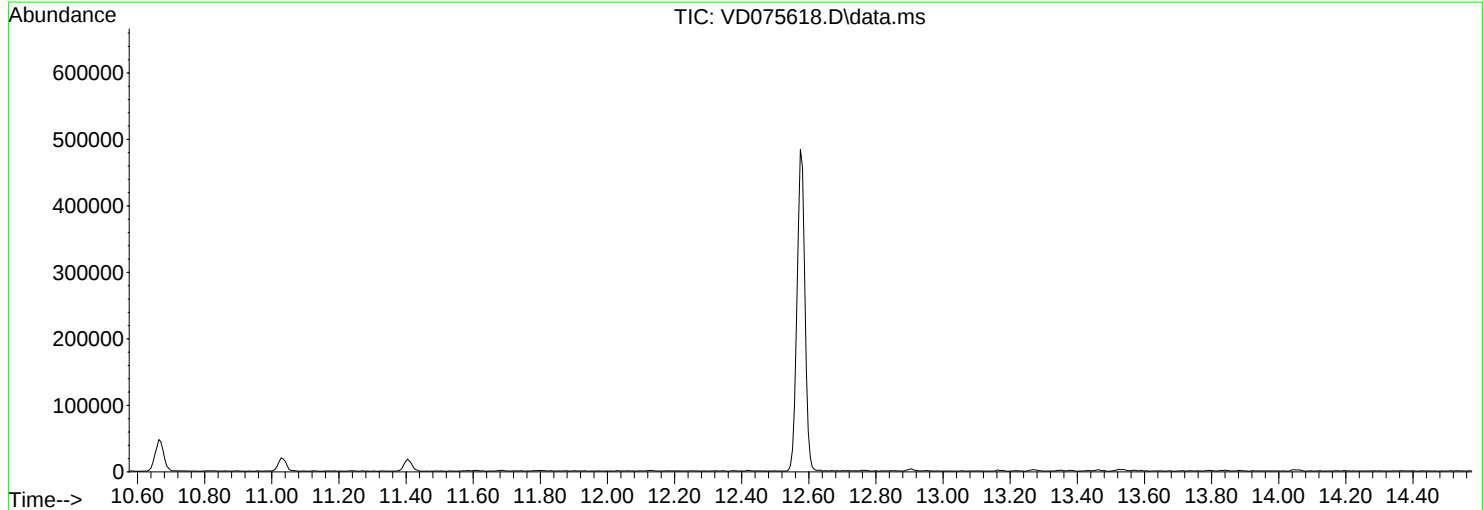

AutoFind: Scans 1867, 1868, 1869; Background Corrected with Scan 1859

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	15.9	13159	PASS
75	95	30	60	47.4	39387	PASS
95	95	100	100	100.0	83011	PASS
96	95	5	9	6.5	5411	PASS
173	174	0.00	2	0.6	512	PASS
174	95	50	100	98.1	81405	PASS
175	174	5	9	7.2	5828	PASS
176	174	95	101	95.1	77376	PASS
177	176	5	9	6.5	5018	PASS